

HiRes Ultra 3D


HASSLE FREE MRI



Introducing

HiRes Ultra 3D

COCHLEAR IMPLANT

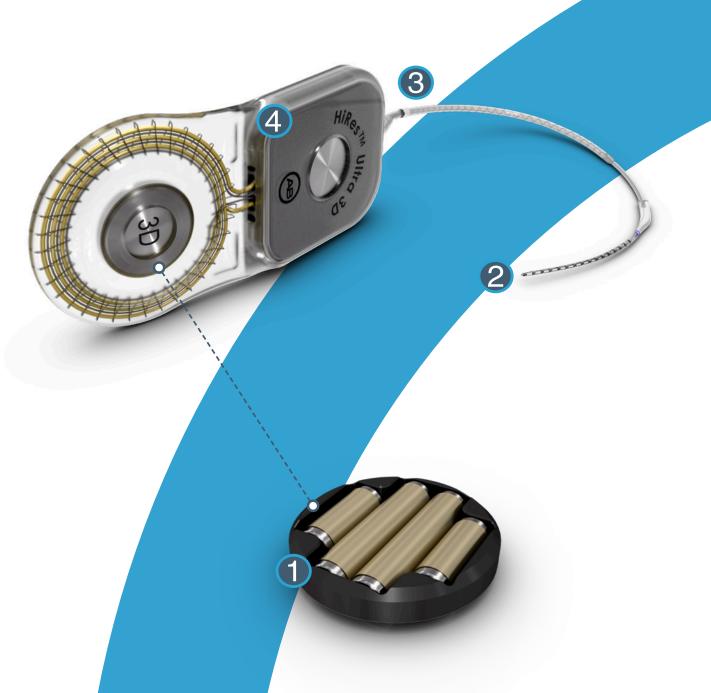

- Hassle Free MRIs: With a unique multi-magnet assembly that provides 3D magnetic field alignment, the HiRes™ Ultra 3D does not require any preparation—such as surgery, head bandaging or restrictions on head orientation—to receive a high-resolution MRI.
- 2. Cochlea Structure Preservation: Both the HiFocus™ SlimJ and the HiFocus™ Mid-Scala electrodes are designed to protect the delicate cochlea structures¹,2,3,4,5 and provide complete coverage of the cochlea for full-spectrum sound.^{6,7}
- 3. Intra-Operative Measurements: HiRes Ultra 3D features a second grounding electrode that can be used for measurements taken in the course of the surgery.
- 4. HiResolution Technology: HiRes Ultra 3D is designed to deliver your patients the proven benefits of hearing clearer speech and a broader range of sounds. Under software control, the 16 independent current sources of the AB implant can steer stimulation to 120 separate locations along the cochlea, thereby increasing the amount of frequency information that can be delivered.⁸




HASSLE FREE MRI

We at Advanced Bionics believe that an MRI procedure should be hassle free for you and your patients. The HiRes Ultra 3D innovative multi-magnet assembly provides alignment to the 3D MRI field, allowing adult and paediatric users to safely undergo high-resolution imaging, such as 3.0 Tesla MRIs, without any preparation, surgery or head bandaging.

This unique multi-magnet assembly is composed of four rotatable magnet rods encased in a revolving frame that allows the magnet to provide alignment with the MRI field in all three dimensions.


If diagnostic procedures require a reduced-image artifact range, the magnet can be easily removed and replaced with a non-magnetic spacer through a small incision made prior to an MRI.

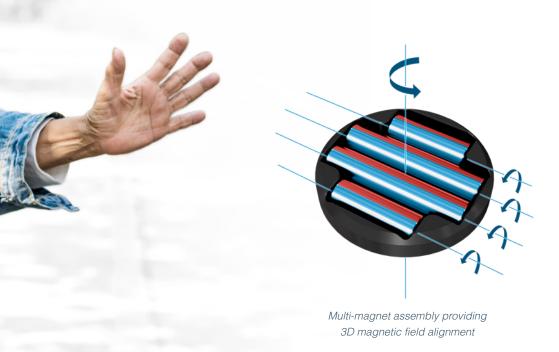

PAIN FREE

Going into an MRI tube is stressful, especially for your young patients. Our HiRes Ultra 3D cochlear implant requires no restriction on head orientation during an MRI, ensuring your patient a truly stress-free MRI experience.

The smooth movement of the multi-magnet assembly generates such low torque that adults and paediatric recipients feel no pain or discomfort due to magnetic pulling during a high-resolution imaging MRI.^{9,10,11,12}

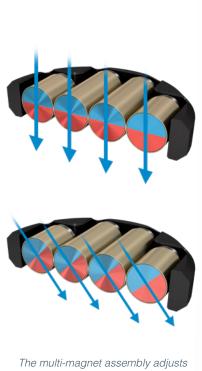

The multi-magnet assembly adjusts to the variations in the magnetic field







UNINTERRUPTED HEARING

Eliminating the lengthy preparation procedures for a CI patient before an MRI saves time and hassle for you and for your patients.

With HiRes Ultra 3D, you don't need any special preparation for an MRI other than to ask your patients to take off their processor. When the scan is done, all they have to do is put their processor back on to return to hearing. With the HiRes Ultra 3D cochlear implant we provide your patients with uninterrupted hearing, which reduces the stress particularly with kids, who then have the ability to hear their parents right before and after the MRI scan.



The HiRes Ultra 3D multi-magnet assembly has been tested to keep working even after two hundred 3.0 Tesla MRI routines¹³

THE FOUNDATION OF BETTER HEARING

Better technology means better hearing, and better hearing leads to better living. That is why every aspect of our HiRes Ultra 3D cochlear implant system has been optimised.

We are passionate about pushing the limits of technology to provide the most complete, natural and reliable hearing solutions possible for your patients.

Every aspect of our hearing technology also includes being gentle on the inner ear. For that reason all our HiFocus[™] structure-preserving electrodes allow for the best possible hearing outcomes.^{1,14,15}



The HiRes Ultra 3D Cochlear Implant has been awarded the Medtech Breakthrough Award 2019 for Best Medical Device Solution.

REFERENCES

- 1. Dietz A, Iso-Mustajärvi M, Sipari S, Tervaniemi J, Gazibegovic D; Evaluation of a new slim lateral wall electrode for cochlear implantation: an imaging study in human temporal bones. Eur Arch Otorhinolaryngol. 2018 Jul;275(7):1723-1729
- 2. Frisch CD, Carlson ML, Lane JI, Driscoll CL; Evaluation of a new mid-scala cochlear implant electrode using microcomputed tomography. Laryngoscope. 2015 Dec:125(12):2778-83
- 3. Hassepass F, Bulla S, Maier W, Laszig R, Arndt S, Beck R, Traser L, Aschendorff A; The New Mid-Scala Electrode Array: A Radiologic And Histologic Study In Human Temporal Bones. Otology & Neurotology 2014; 35(8):1415-20
- 4. Dietz A, Gazibegovic D, Tervaniemi J, Vartiainen VM, Löppönen H; Insertion characteristics and placement of the Mid-Scala electrode array in human temporal bones using detailed cone beam computed tomography. Eur Arch Otorhinolaryngol. 2016 Dec;273(12):4135-4143
- 5. Benghalem A, Gazibegovic D, Saadi F, Tazi-Chaoui Z; Use of a mid-scala and a lateral wall electrode in children: insertion depth and hearing preservation.

 Acta Otolaryngol. 2017 Jan;137(1):1-7
- 6. Olga Stakhovskaya, corresponding author Divya Sridhar, Ben H. Bonham, and Patricia A. Leake; Frequency Map for the Human Cochlear Spiral Ganglion: Implications for Cochlear Implants. J Assoc Res Otolaryngol. 2007 Jun; 8(2): 220–233
- 7. Avci E, Nauwelaers T, Lenarz T, Hamacher V, Kral A; Variations in microanatomy of the human cochlea. J Comp Neurol. 2014 Oct 1; 522(14): 3245–3261
- 8. Koch D. B., Downing M., Osberger M. J., and Litvak L. (2007). "Using current steering to increase spectral resolution in CII and HiRes 90K users," Ear Hear. 28(2)
- 9. Grossi, DB, et al. Pressure pain threshold in the craniocervical muscles of women with episodic and chronic migraine, Arq Neuropsiquiatr. 69(4):607-12, Aug 2011
- 10. Antonaci, F, et al. Pressure Algometry in Healthy Subjects: Inter-Examiner Variability. Scandinavian Journal of Rehabilitation Medicine, 30, 1998
- 11. Antonaci, F, et al. Pain threshold in humans. A study with the pressure algometer. Functional Neurology, 7(4) 1992
- 12. Ferracini, GN. A Comparison Pressure Pain Threshold in Pericranial and Extracephalic Regions in Children with Migraine. Pain Medicine, 15, 2014
- 13. Internal testing. Data on file.
- 14. Gazibegovic D, Bero EM; Multicenter surgical experience evaluation on the Mid-Scala electrode and insertion tools. Eur Arch Otorhinolaryngol. 2017 Feb;274(2):1147-1151
- 15. Boyle PJ; The rational for a mid-scala electrode array. Eur Ann Otorhinolaryngol Head Neck Dis. 2016 Jun



ADVANCED BIONICS LLC – 28515 Westinghouse Place - Valencia, CA 91355, United States T: +1.877.829.0026 - T: +1.661.362.1400 - F: +1.661.362.1500 *info.us@advancedbionics.com*

EC REP ADVANCED BIONICS GMBH - Feodor-Lynen-Strasse 35 – 30625 Hannover, Germany

ADVANCED BIONICS UK & EIRE, 2 Breaks House, Mill Court, Great Shelford, Cambridge, CB22 5LD, UK T: +44.1223.847.888 - F: +44.1223.847.898 info.uk@advancedbionics.com

For information on additional AB locations, please visit advancedbionics.com/contact

Advanced Bionics - A Sonova brand

Please contact your local AB representative for regulatory approval and availability in your region.

