ADVANCED BIONICS
POWERFUL CONNECTIONS

Reliability Report July 2026

IMPLANTABLE COCHLEAR STIMULATORS AND SOUND PROCESSORS

A Sonova brand

POWERFUL CONNECTIONS START HERE

ADVANCED BIONICS
POWERFUL CONNECTIONS

A Sonova brand

TRANSPARENCY IS THE FOUNDATION OF TRUST

With our annual product reliability report, we reaffirm our commitment to quality and integrity for our valued patients and partners.

Alistair Simpson
PRESIDENT, ADVANCED BIONICS

HIRES ULTRA 3D V2

NUMBER OF REGISTERED HIRES ULTRA 3D V2 IMPLANTS

As of April 1, 2026.
Date of first commercial introduction: 2019.[a]

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	37316	12124	49440[b]
ANSI/AAMI CI86	39722[c]	9718	49440

Number of registered users is detailed for adults, children (defined as less than 18 years at implantation by ISO 5841, and less than 10 years at implantation by CI86), and a combination of all ages in accordance with reporting methodologies.

a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

Graph title shows the reporting standard

ISO 5841-2:2014

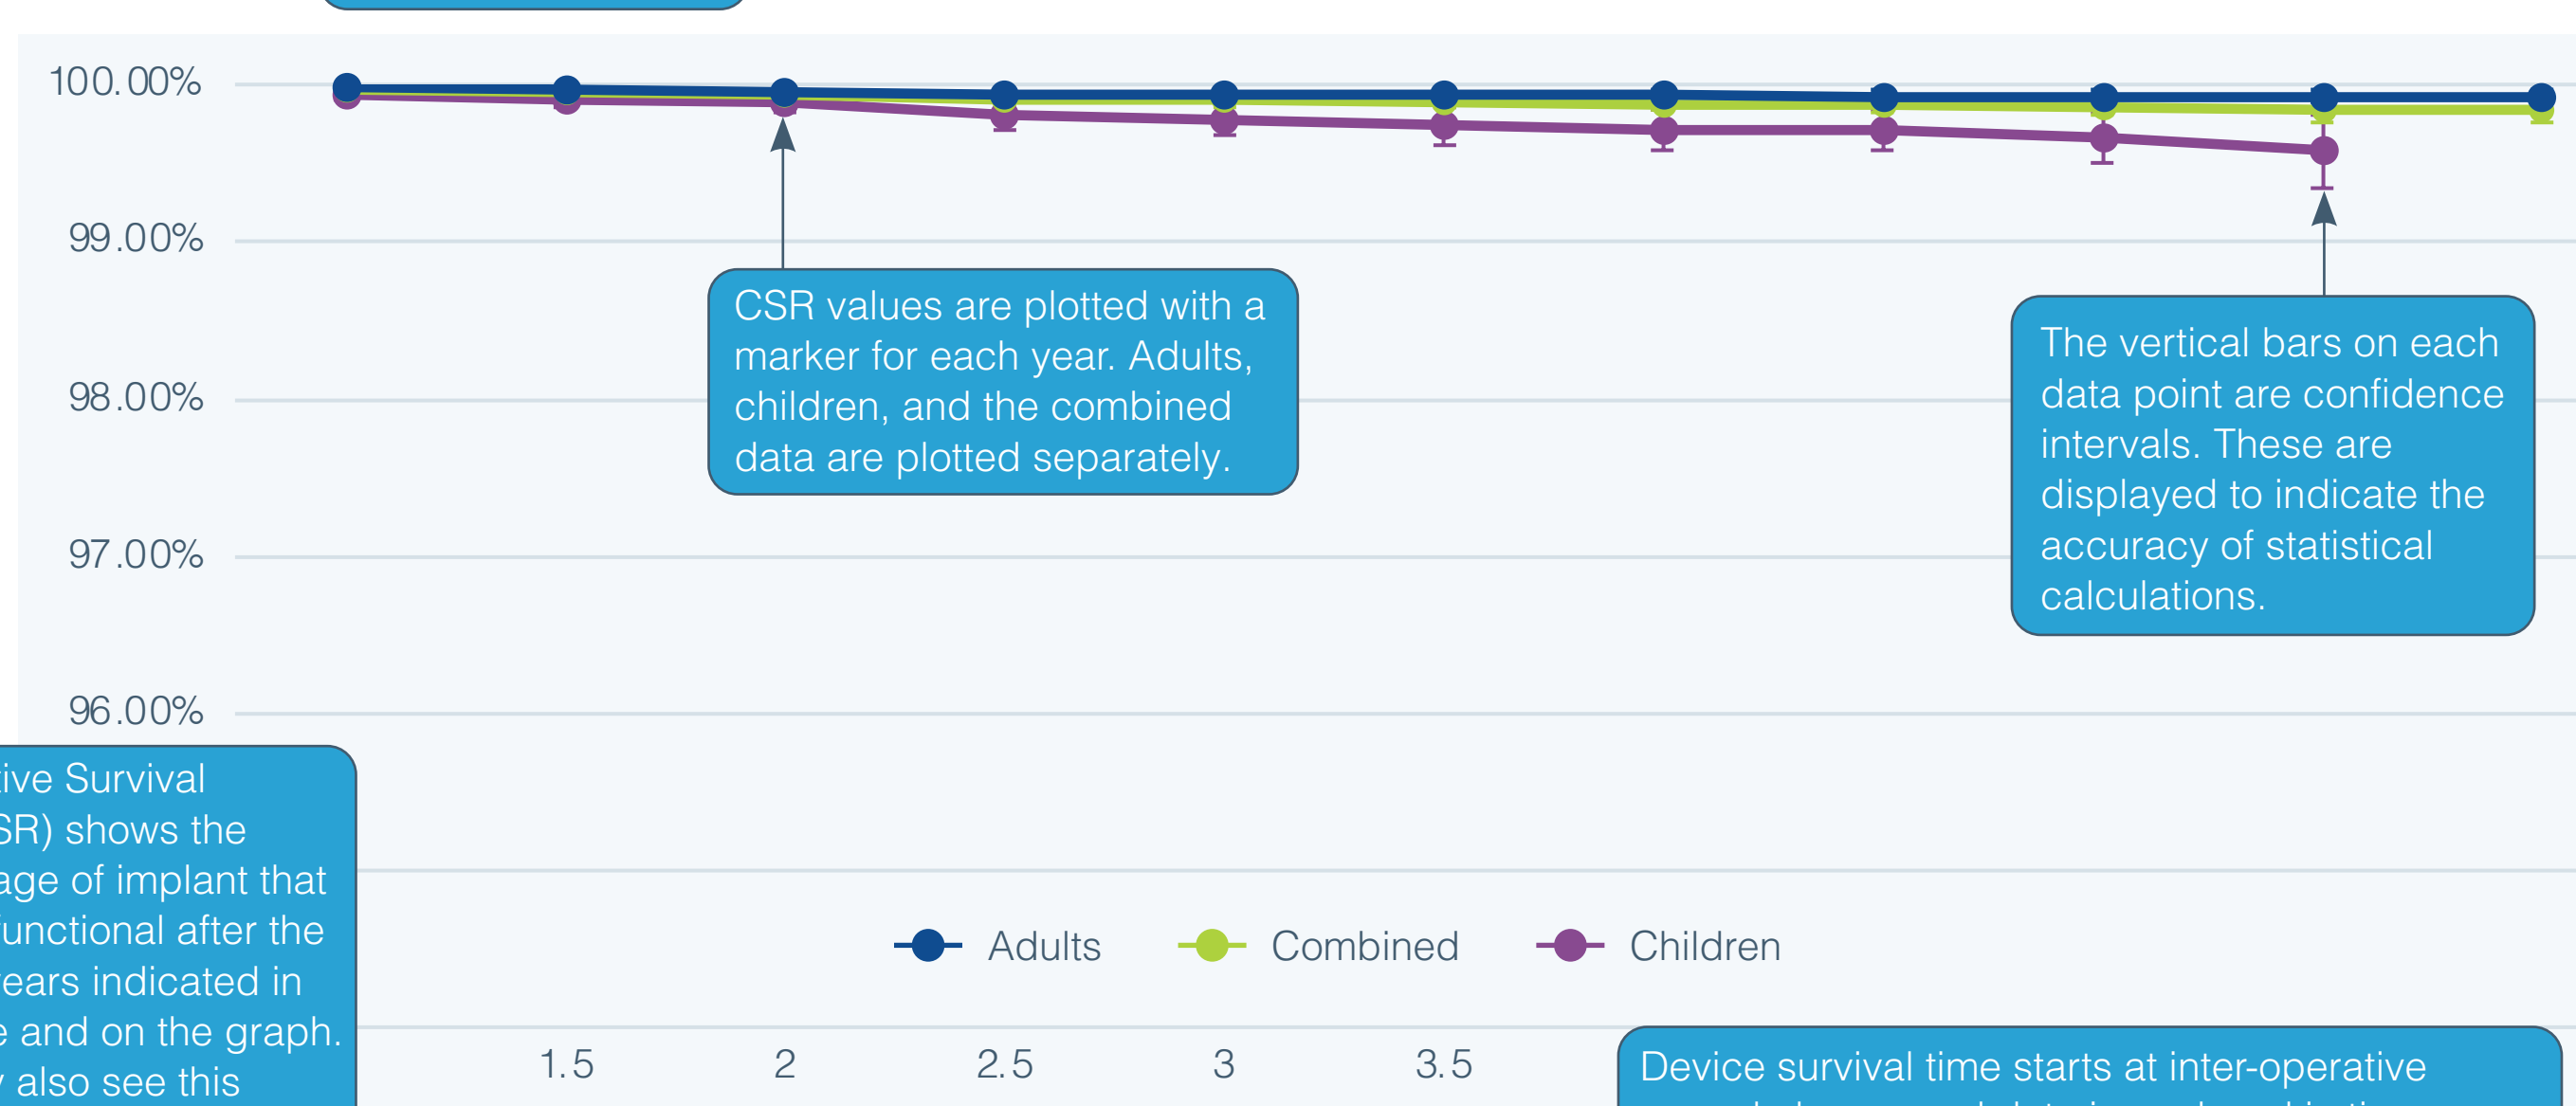

CSR values are plotted with a marker for each year. Adults, children, and the combined data are plotted separately.

The vertical bars on each data point are confidence intervals. These are displayed to indicate the accuracy of statistical calculations.

Cumulative Survival Rate (CSR) shows the percentage of implant that are still functional after the time in years indicated in the table and on the graph. You may also see this described as Cumulative Survival Percentage.

Device survival time starts at inter-operative wound closure and data is analyzed in time intervals according to the standard.

CUMULATIVE SURVIVAL RATE

Years in use	1	1.5	2	2.5	3	3.5	4	4.5	5	5.5	6
ADULTS	99.98%	99.96%	99.96%	99.95%	99.94%	99.94%	99.94%	99.93%	99.93%	99.93%	99.93%
COMBINED	99.97%	99.95%	99.94%	99.91%	99.90%	99.89%	99.88%	99.87%	99.86%	99.83%	99.83%
CHILDREN	99.94%	99.91%	99.89%	99.81%	99.78%	99.74%	99.71%	99.71%	99.66%	99.58%	N/A*

Detailed CSR percentages are shown for each year in the table. Results are shown as: adult, children and combined total.

*Sample size is not large enough for reporting.

Graph title shows the reporting standard

ANSI/AAMI CI86

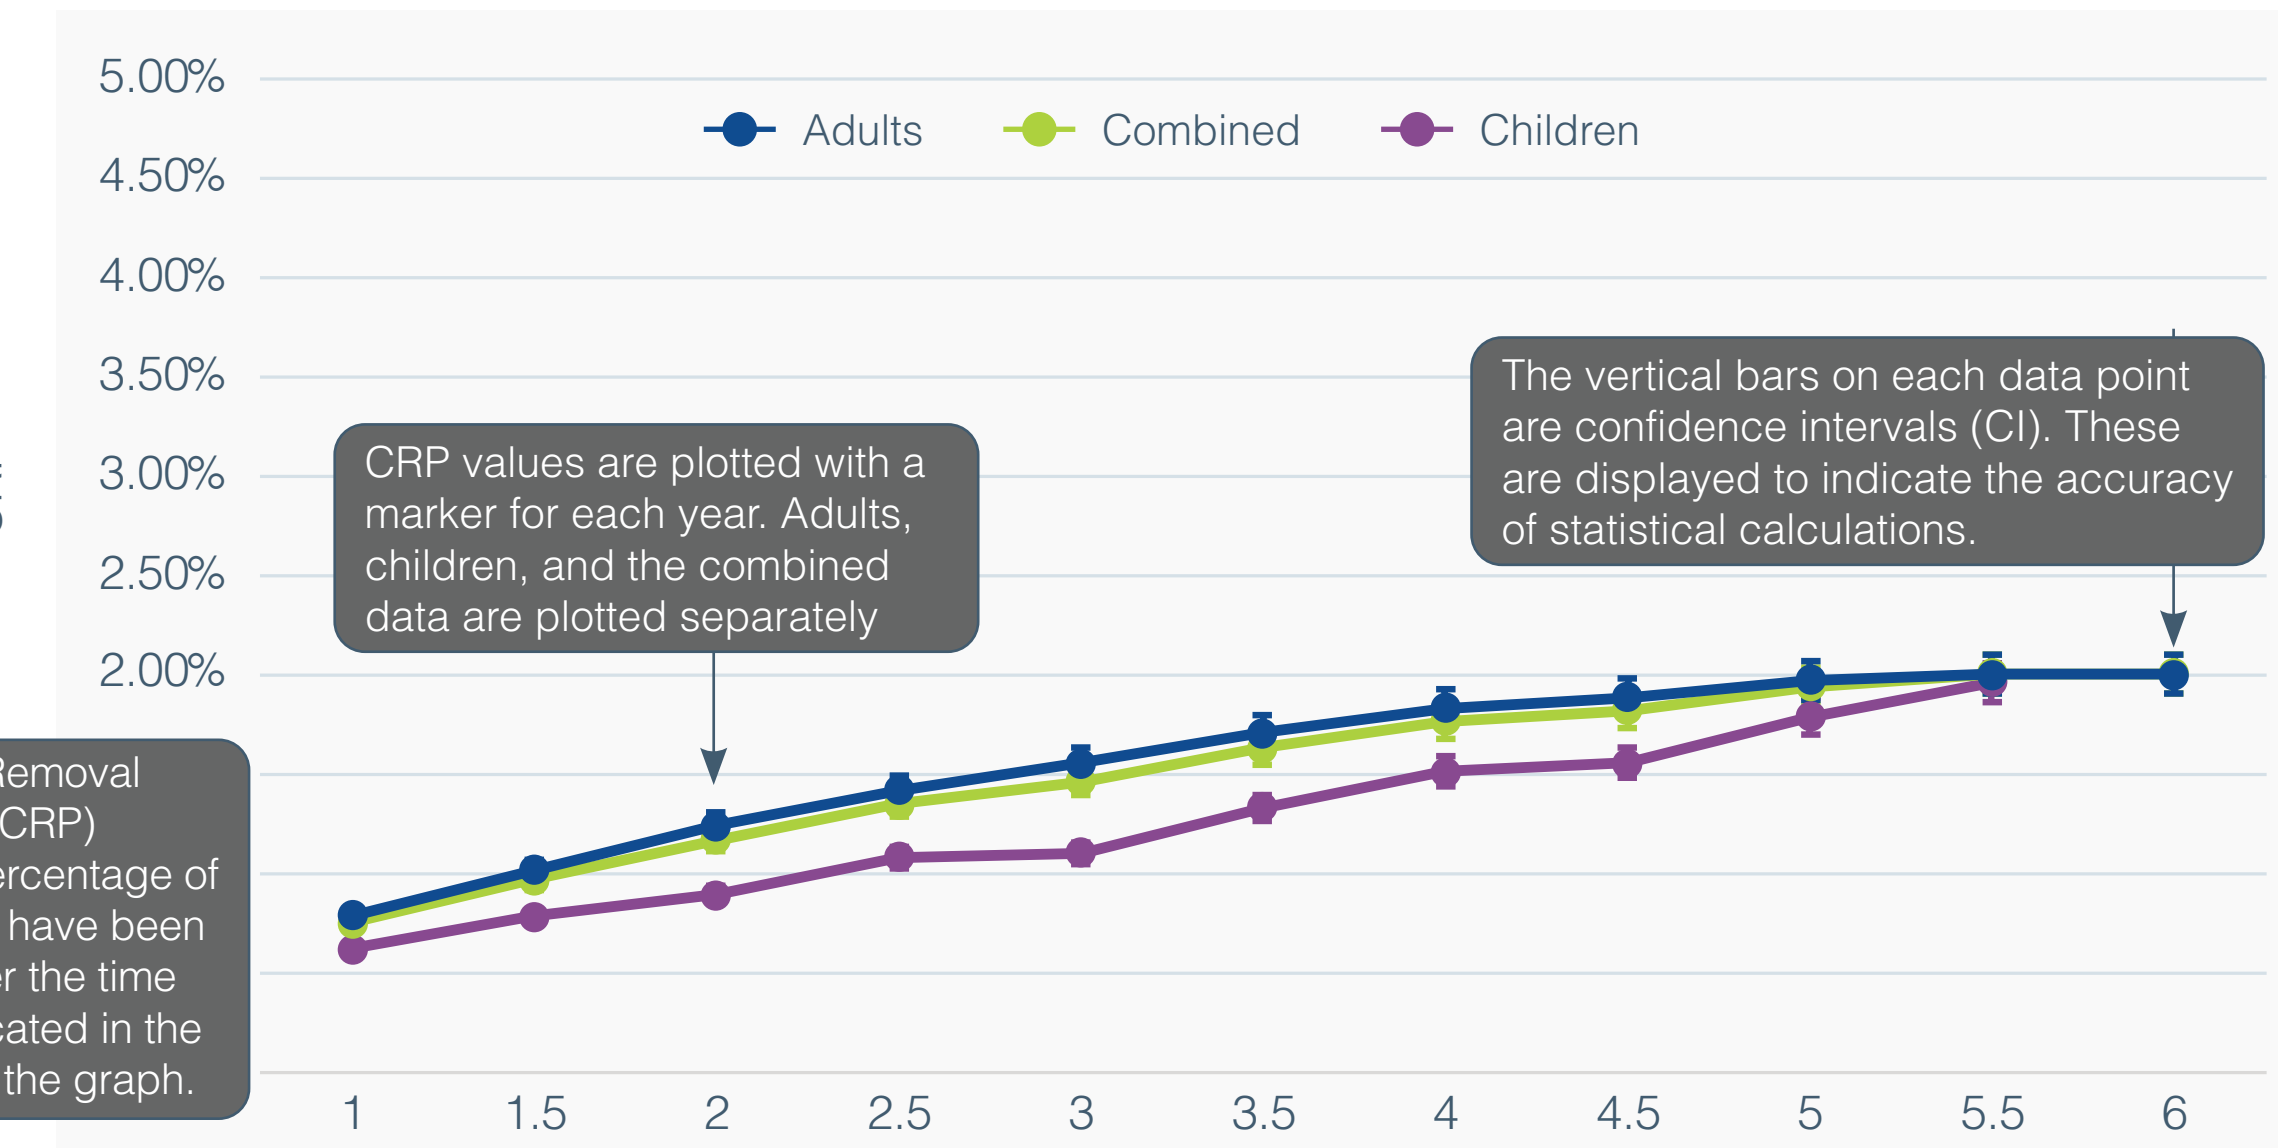

CRP values are plotted with a marker for each year. Adults, children, and the combined data are plotted separately

The vertical bars on each data point are confidence intervals (CI). These are displayed to indicate the accuracy of statistical calculations.

Cumulative Removal Percentage (CRP) shows the percentage of implants that have been removed after the time in years indicated in the table and on the graph.

Device survival time starts at inter-operative wound closure and data is analyzed in time intervals according to the standard.

The ANSI/AAMI CI86 Standard requires that all removed devices are classified into three categories based on the rationale for explantation: device failure, medical reason, or inconclusive.

COMBINED ADULT AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	Total CI Lower
1	0.72%	0.02%	0.01%	0.75%	0.83%	0.67%
1.5	0.92%	0.04%	0.01%	0.97%	1.06%	0.88%
2	1.11%	0.05%	0.01%	1.17%	1.28%	1.07%
2.5	1.26%	0.08%	0.01%	1.35%	1.47%	1.24%
3	1.36%	0.09%	0.02%	1.46%	1.59%	1.34%
3.5	1.52%	0.10%	0.02%	1.63%	1.77%	1.50%
4	1.65%	0.10%	0.02%	1.77%	1.92%	1.62%
4.5	1.70%	0.10%	0.02%	1.82%	1.98%	1.67%
5	1.80%	0.12%	0.02%	1.95%	2.12%	1.77%
5.5	1.85%	0.14%	0.02%	2.01%	2.20%	1.82%
6	1.85%	0.14%	0.02%	2.01%	2.20%	1.82%

Throughout this report, we will present the date and graphs to represent the conditions for: analysis by category for adults and children; removal rates by analysis category for adults and children, and all analysis categories for adults and children combined.

Please see the **Appendix** for a complete data set.

HIRES ULTRA 3D V2

The HiRes™ Ultra 3D (V2) cochlear implant is an update to the previous HiRes Ultra 3D (V1) device. Based off the standard HiRes Ultra platform but featuring an innovative multi-magnet assembly, the HiRes Ultra 3D V2 implant allows the use of clinical MRI at 1.5T and 3T without the need for magnet removal or head-bandaging. Due to the low torque, the recipient can be expected to have a hassle free and pain free experience.

The HiRes Ultra 3D (V2) device has a Cumulative Survival Rate (CSR) of 99.83%.

NUMBER OF REGISTERED HIRES ULTRA 3D V2 IMPLANTS

As of April 1, 2026.
Date of first commercial introduction: 2019.[a]

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	37316	12124	49440[b]
ANSI/AAMI CI86	39722[c]	9718	49440

a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

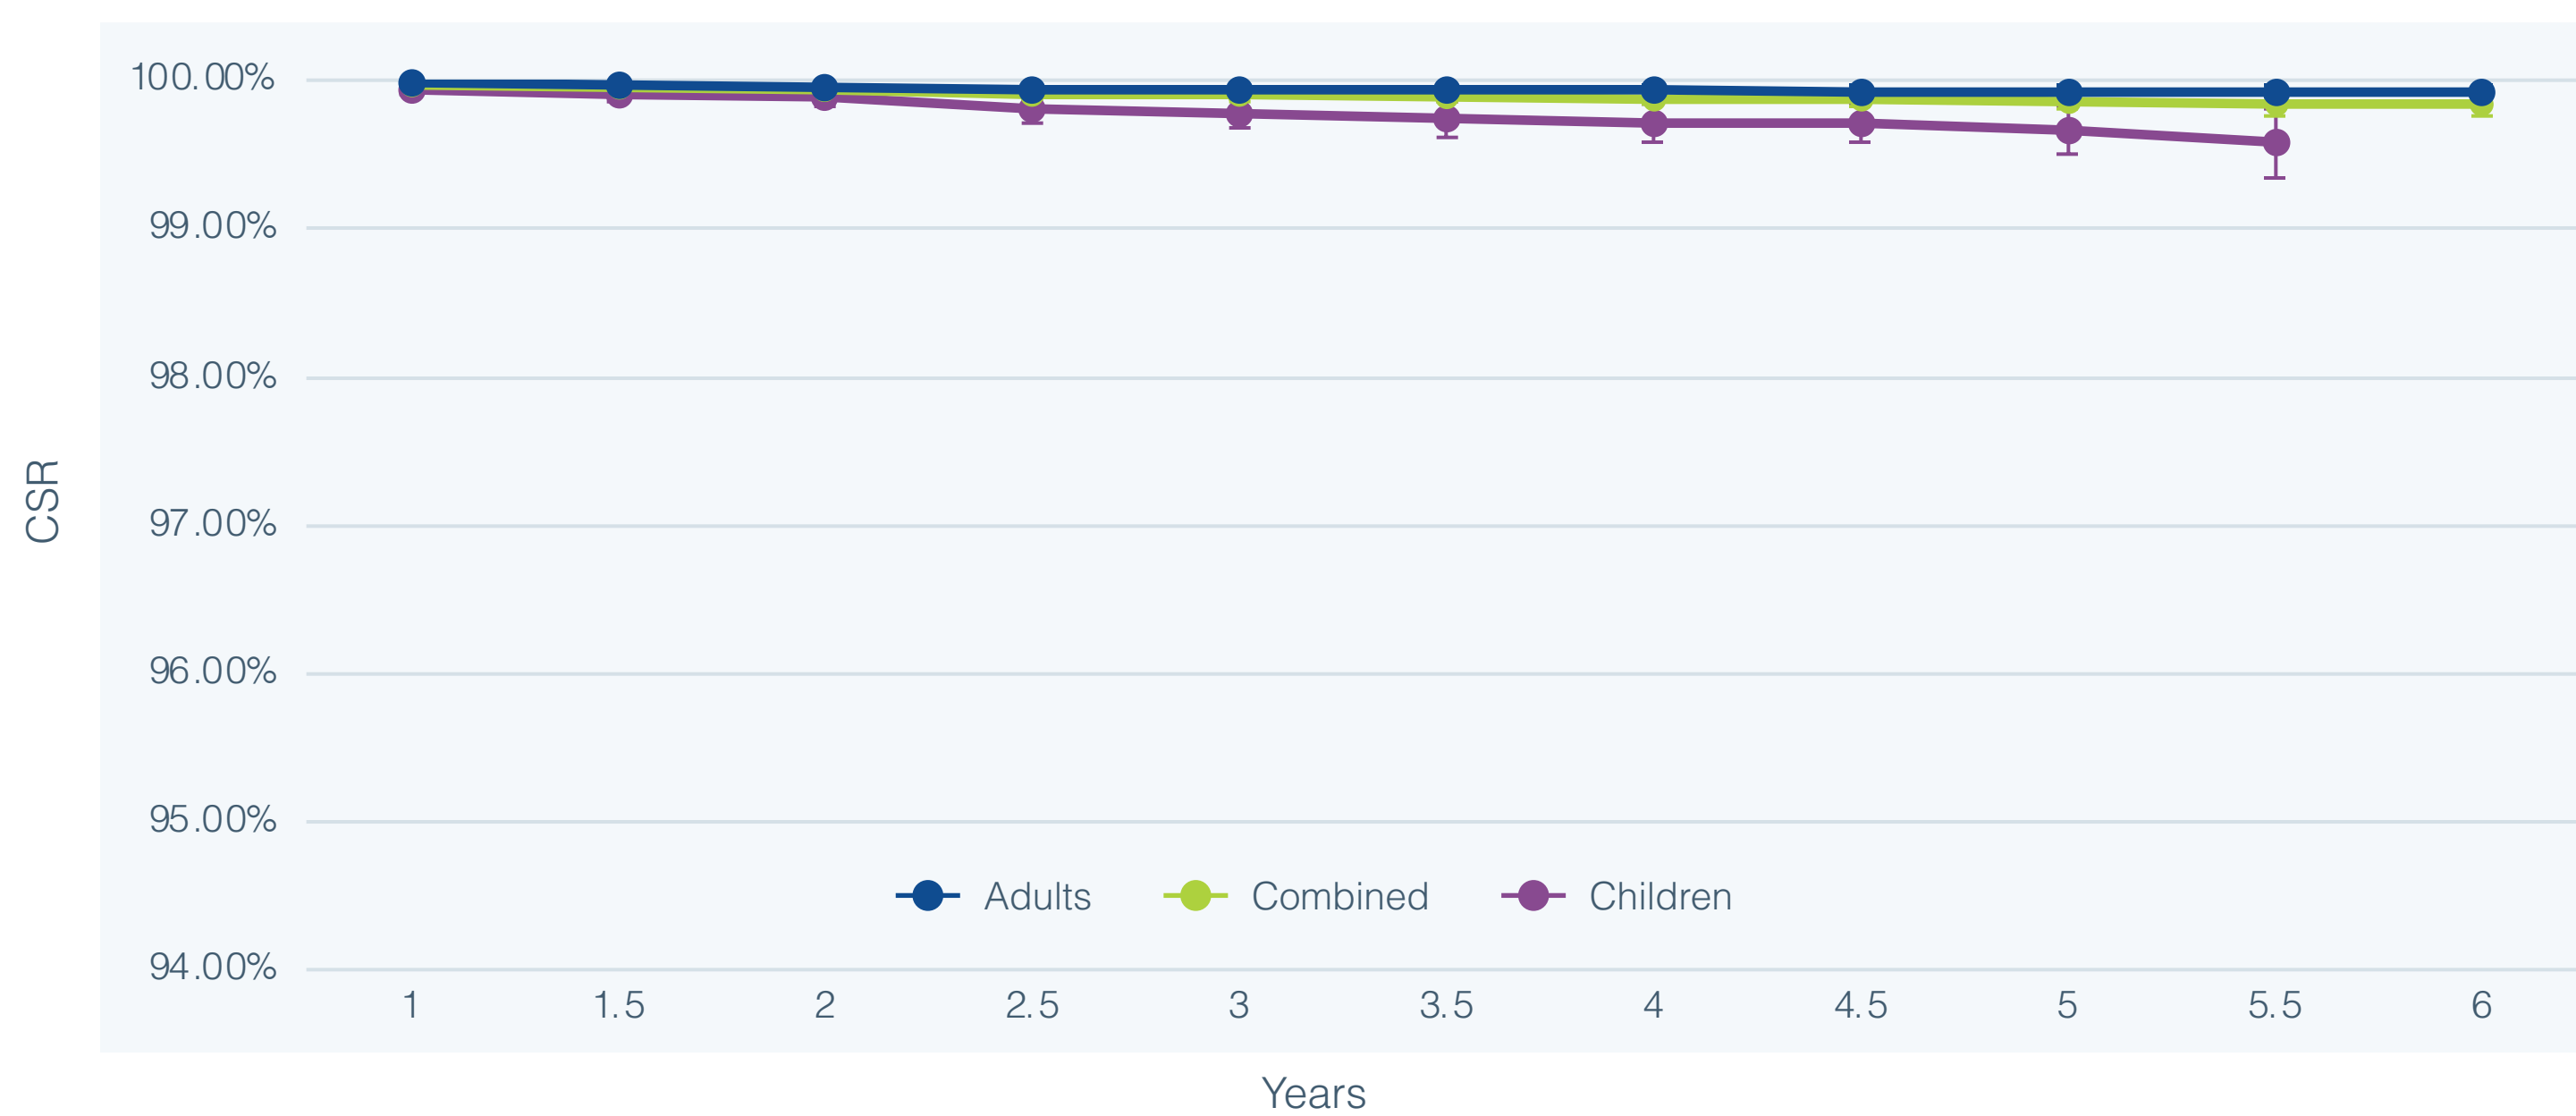

CUMULATIVE SURVIVAL RATE

Years in use	1	1.5	2	2.5	3	3.5	4	4.5	5	5.5	6
ADULTS	99.98%	99.96%	99.96%	99.95%	99.94%	99.94%	99.94%	99.93%	99.93%	99.93%	99.93%
COMBINED	99.97%	99.95%	99.94%	99.91%	99.90%	99.89%	99.88%	99.87%	99.86%	99.83%	99.83%
CHILDREN	99.94%	99.91%	99.89%	99.81%	99.78%	99.74%	99.71%	99.71%	99.66%	99.58%	N/A*

*Sample size is not large enough for reporting.

ANSI/AAMI CI86

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

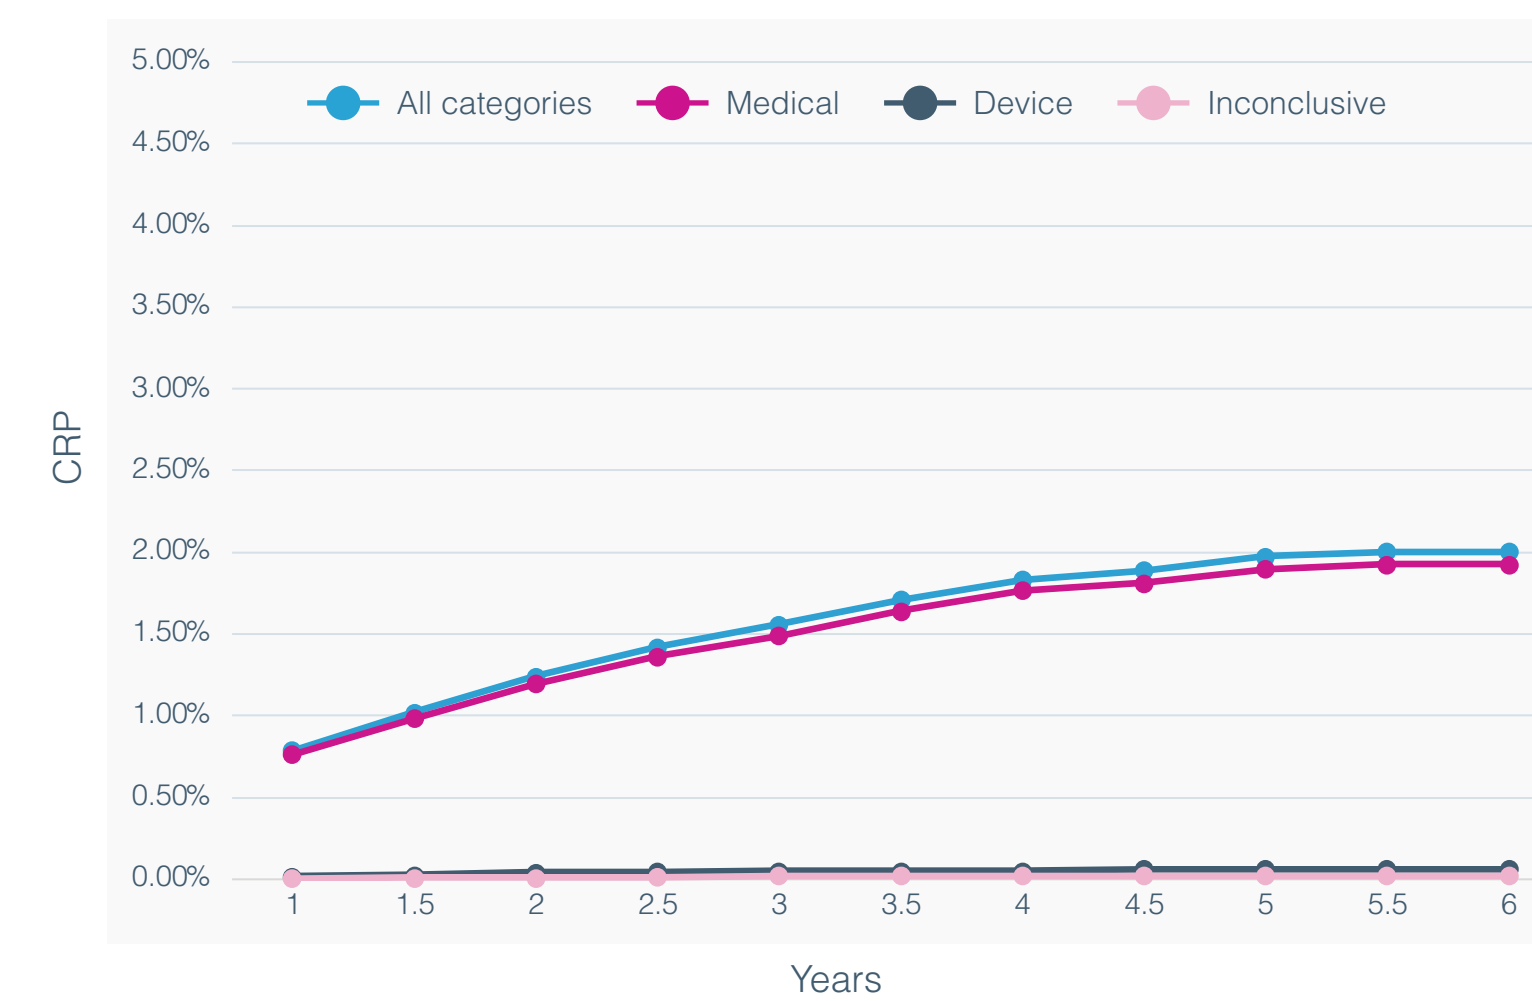

REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

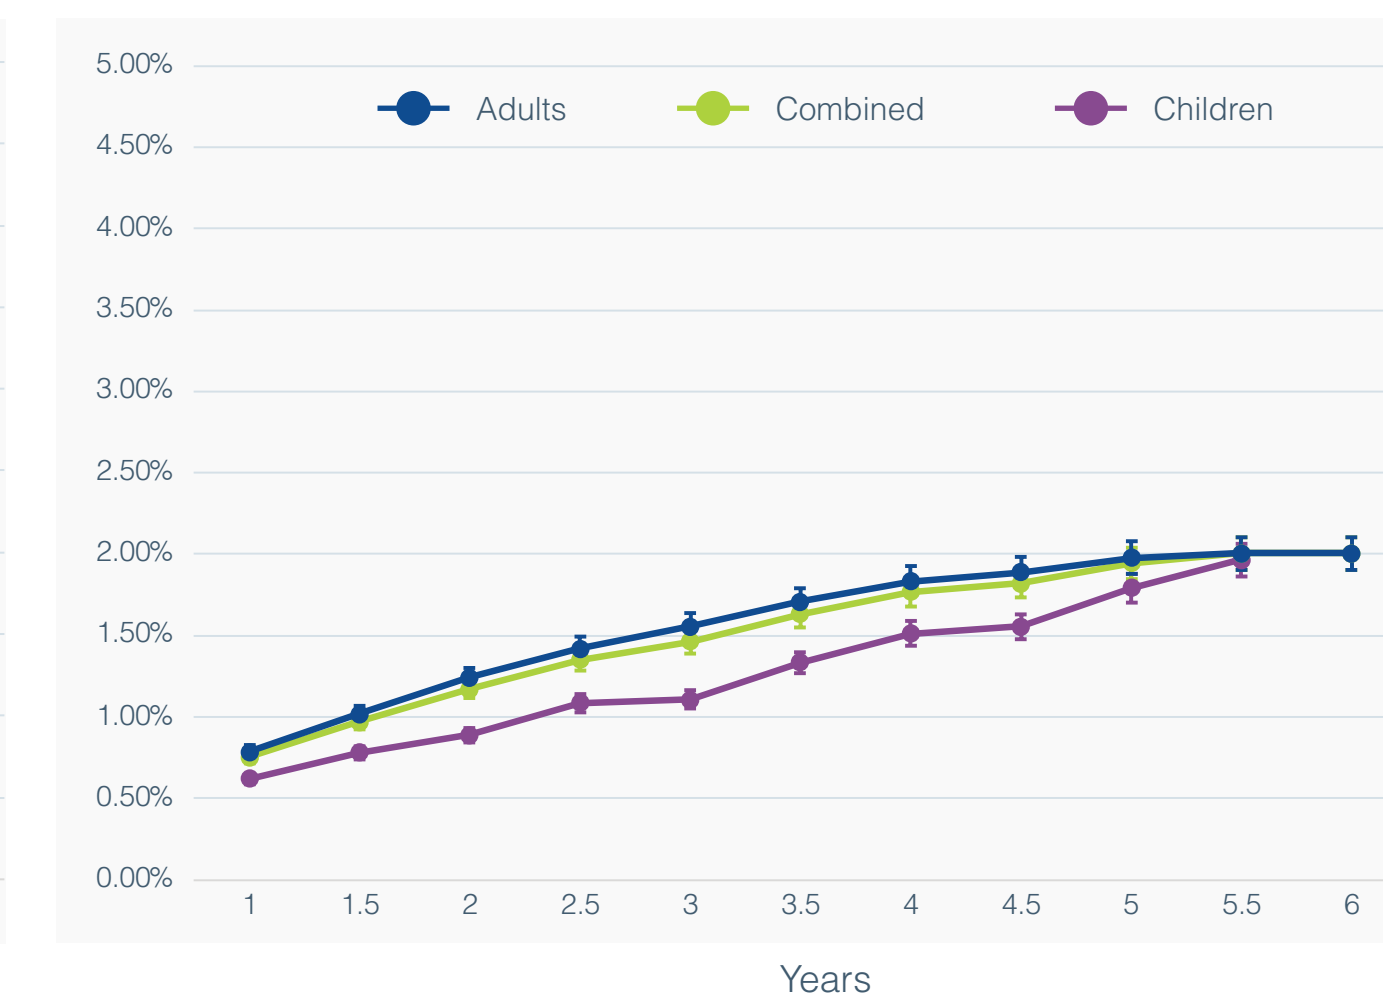

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

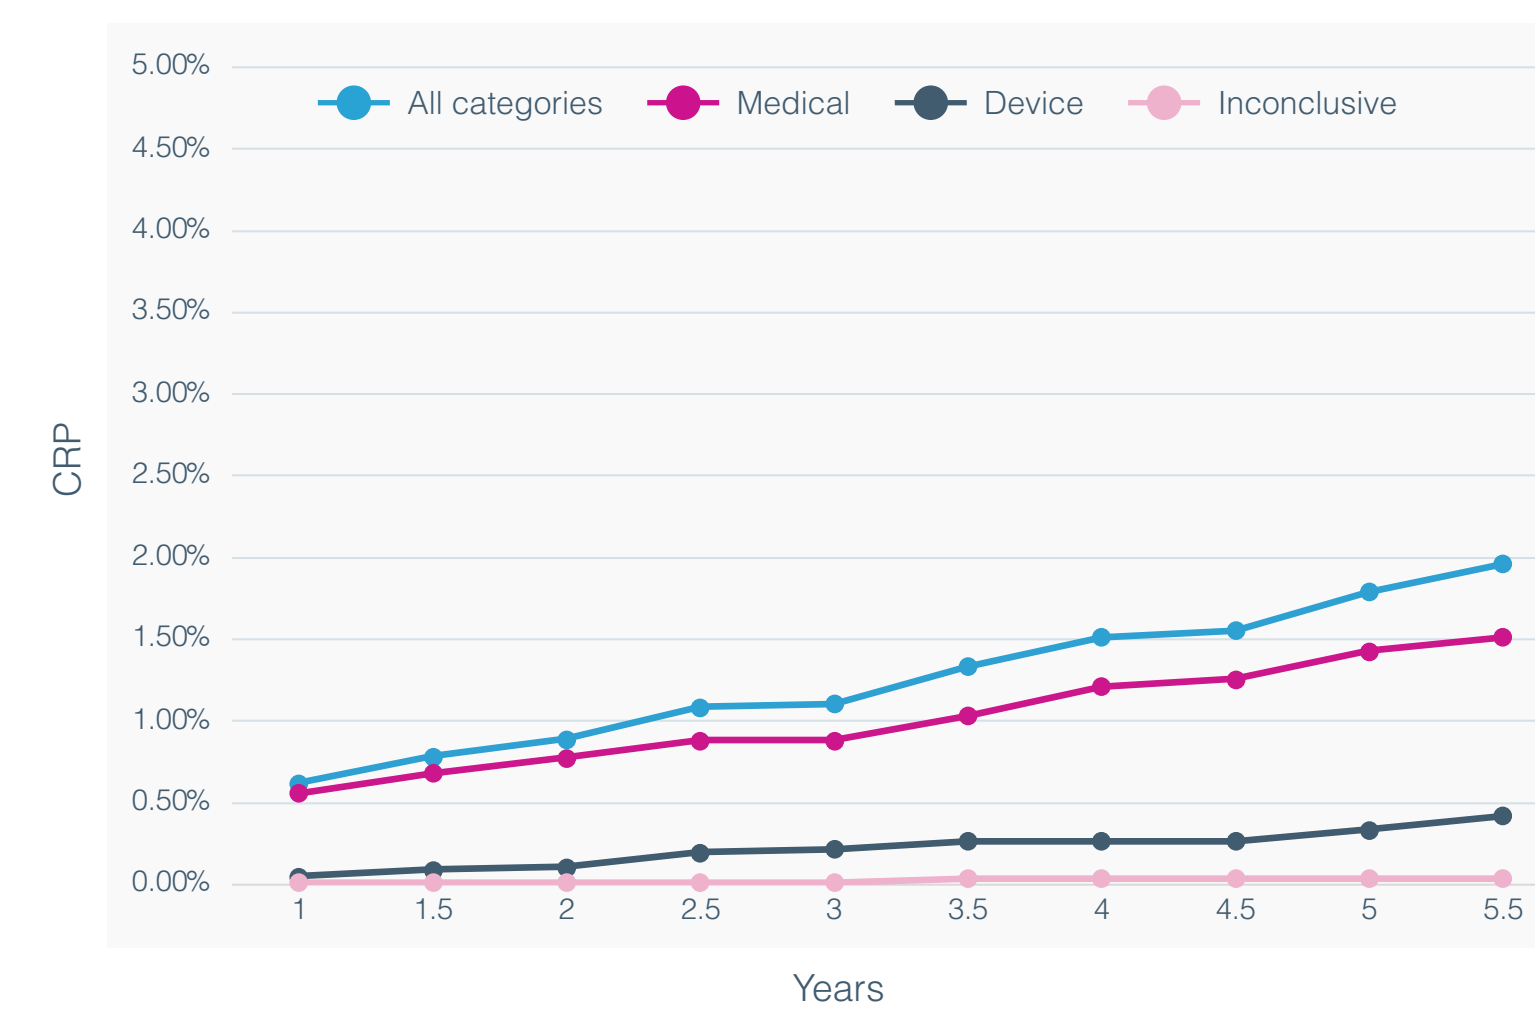

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

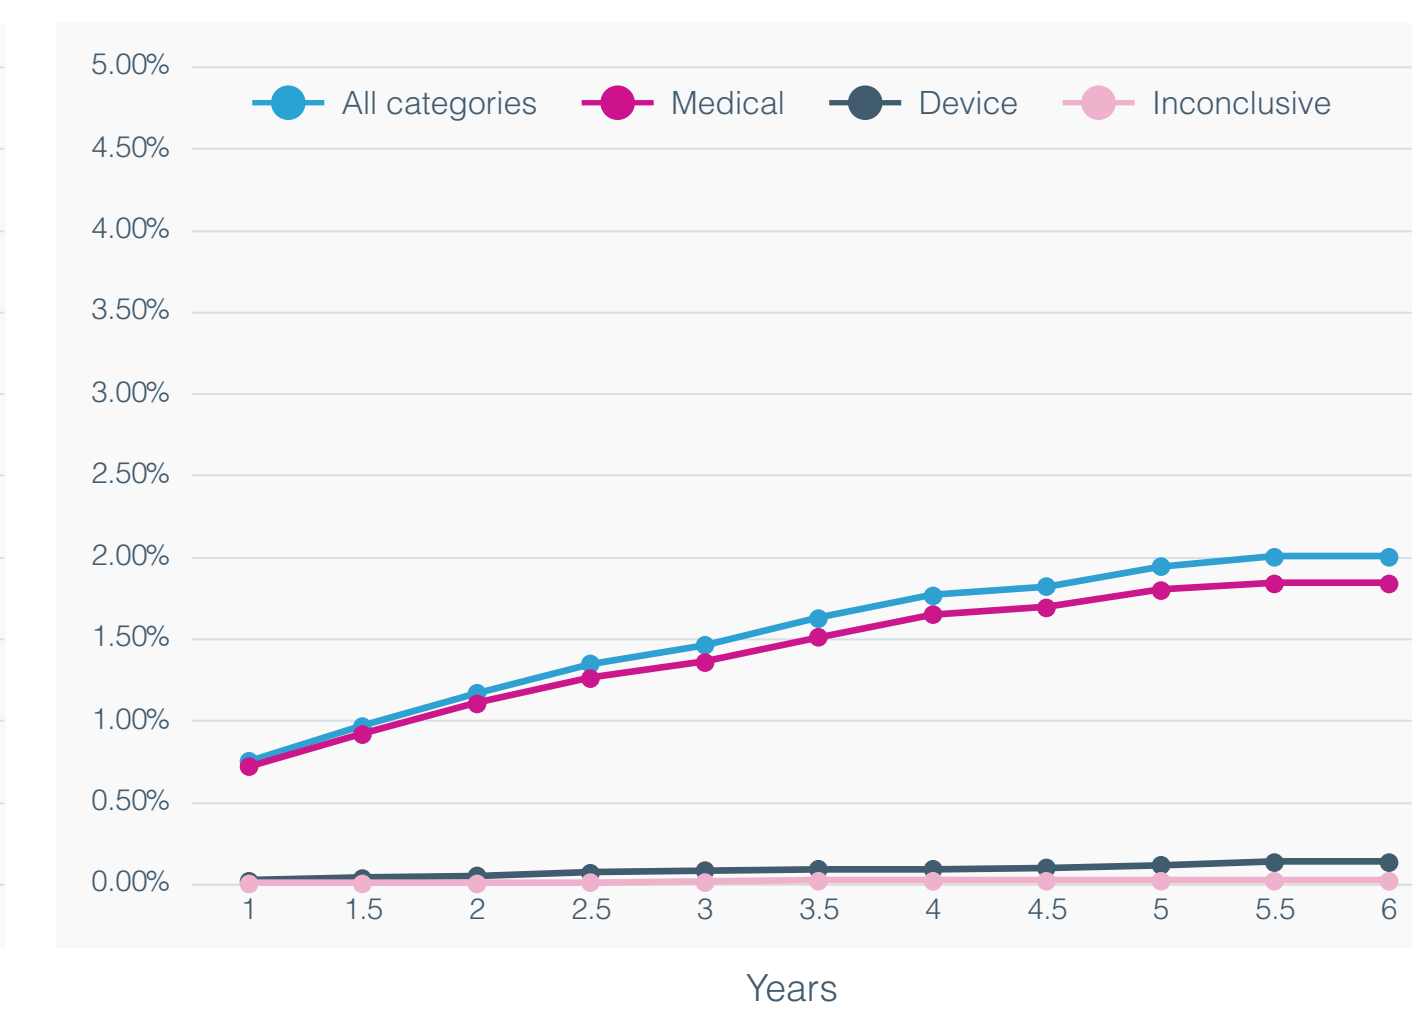

COMBINED ADULT AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	CI Lower
1	0.72%	0.02%	0.01%	0.75%	0.83%	0.67%
1.5	0.92%	0.04%	0.01%	0.97%	1.06%	0.88%
2	1.11%	0.05%	0.01%	1.17%	1.28%	1.07%
2.5	1.26%	0.08%	0.01%	1.35%	1.47%	1.24%
3	1.36%	0.09%	0.02%	1.46%	1.59%	1.34%
3.5	1.52%	0.10%	0.02%	1.63%	1.77%	1.50%
4	1.65%	0.10%	0.02%	1.77%	1.92%	1.62%
4.5	1.70%	0.10%	0.02%	1.82%	1.98%	1.67%
5	1.80%	0.12%	0.02%	1.95%	2.12%	1.77%
5.5	1.85%	0.14%	0.02%	2.01%	2.20%	1.82%
6	1.85%	0.14%	0.02%	2.01%	2.20%	1.82%

Please see the **Appendix** for a complete data set.

HIRES ULTRA V2

Featuring the proven performance platform as the HiRes 90K™ Advantage, the HiRes Ultra (V2) offers a robust, thin, and discreet mechanical design that is suitable for adults and children.

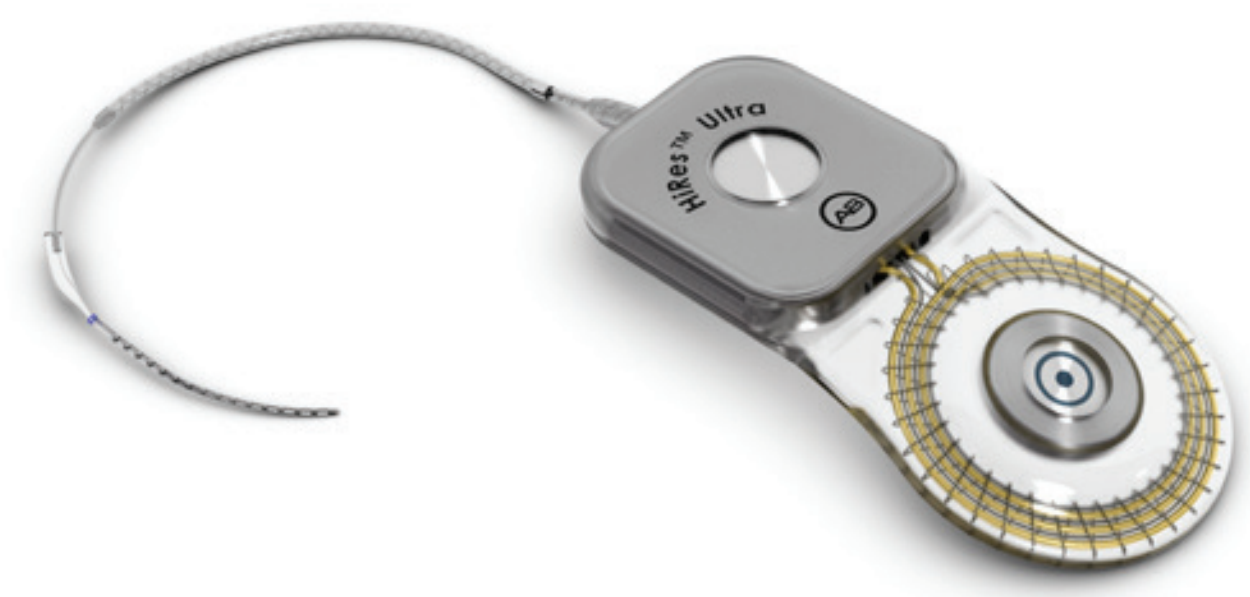

NUMBER OF REGISTERED HIRES ULTRA V2 IMPLANTS

As of April 1, 2026 .
Date of first commercial introduction: 2019.[a]

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	5940	10432	16372[b]
ANSI/AAMI CI86	9174[c]	7198	16372

a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

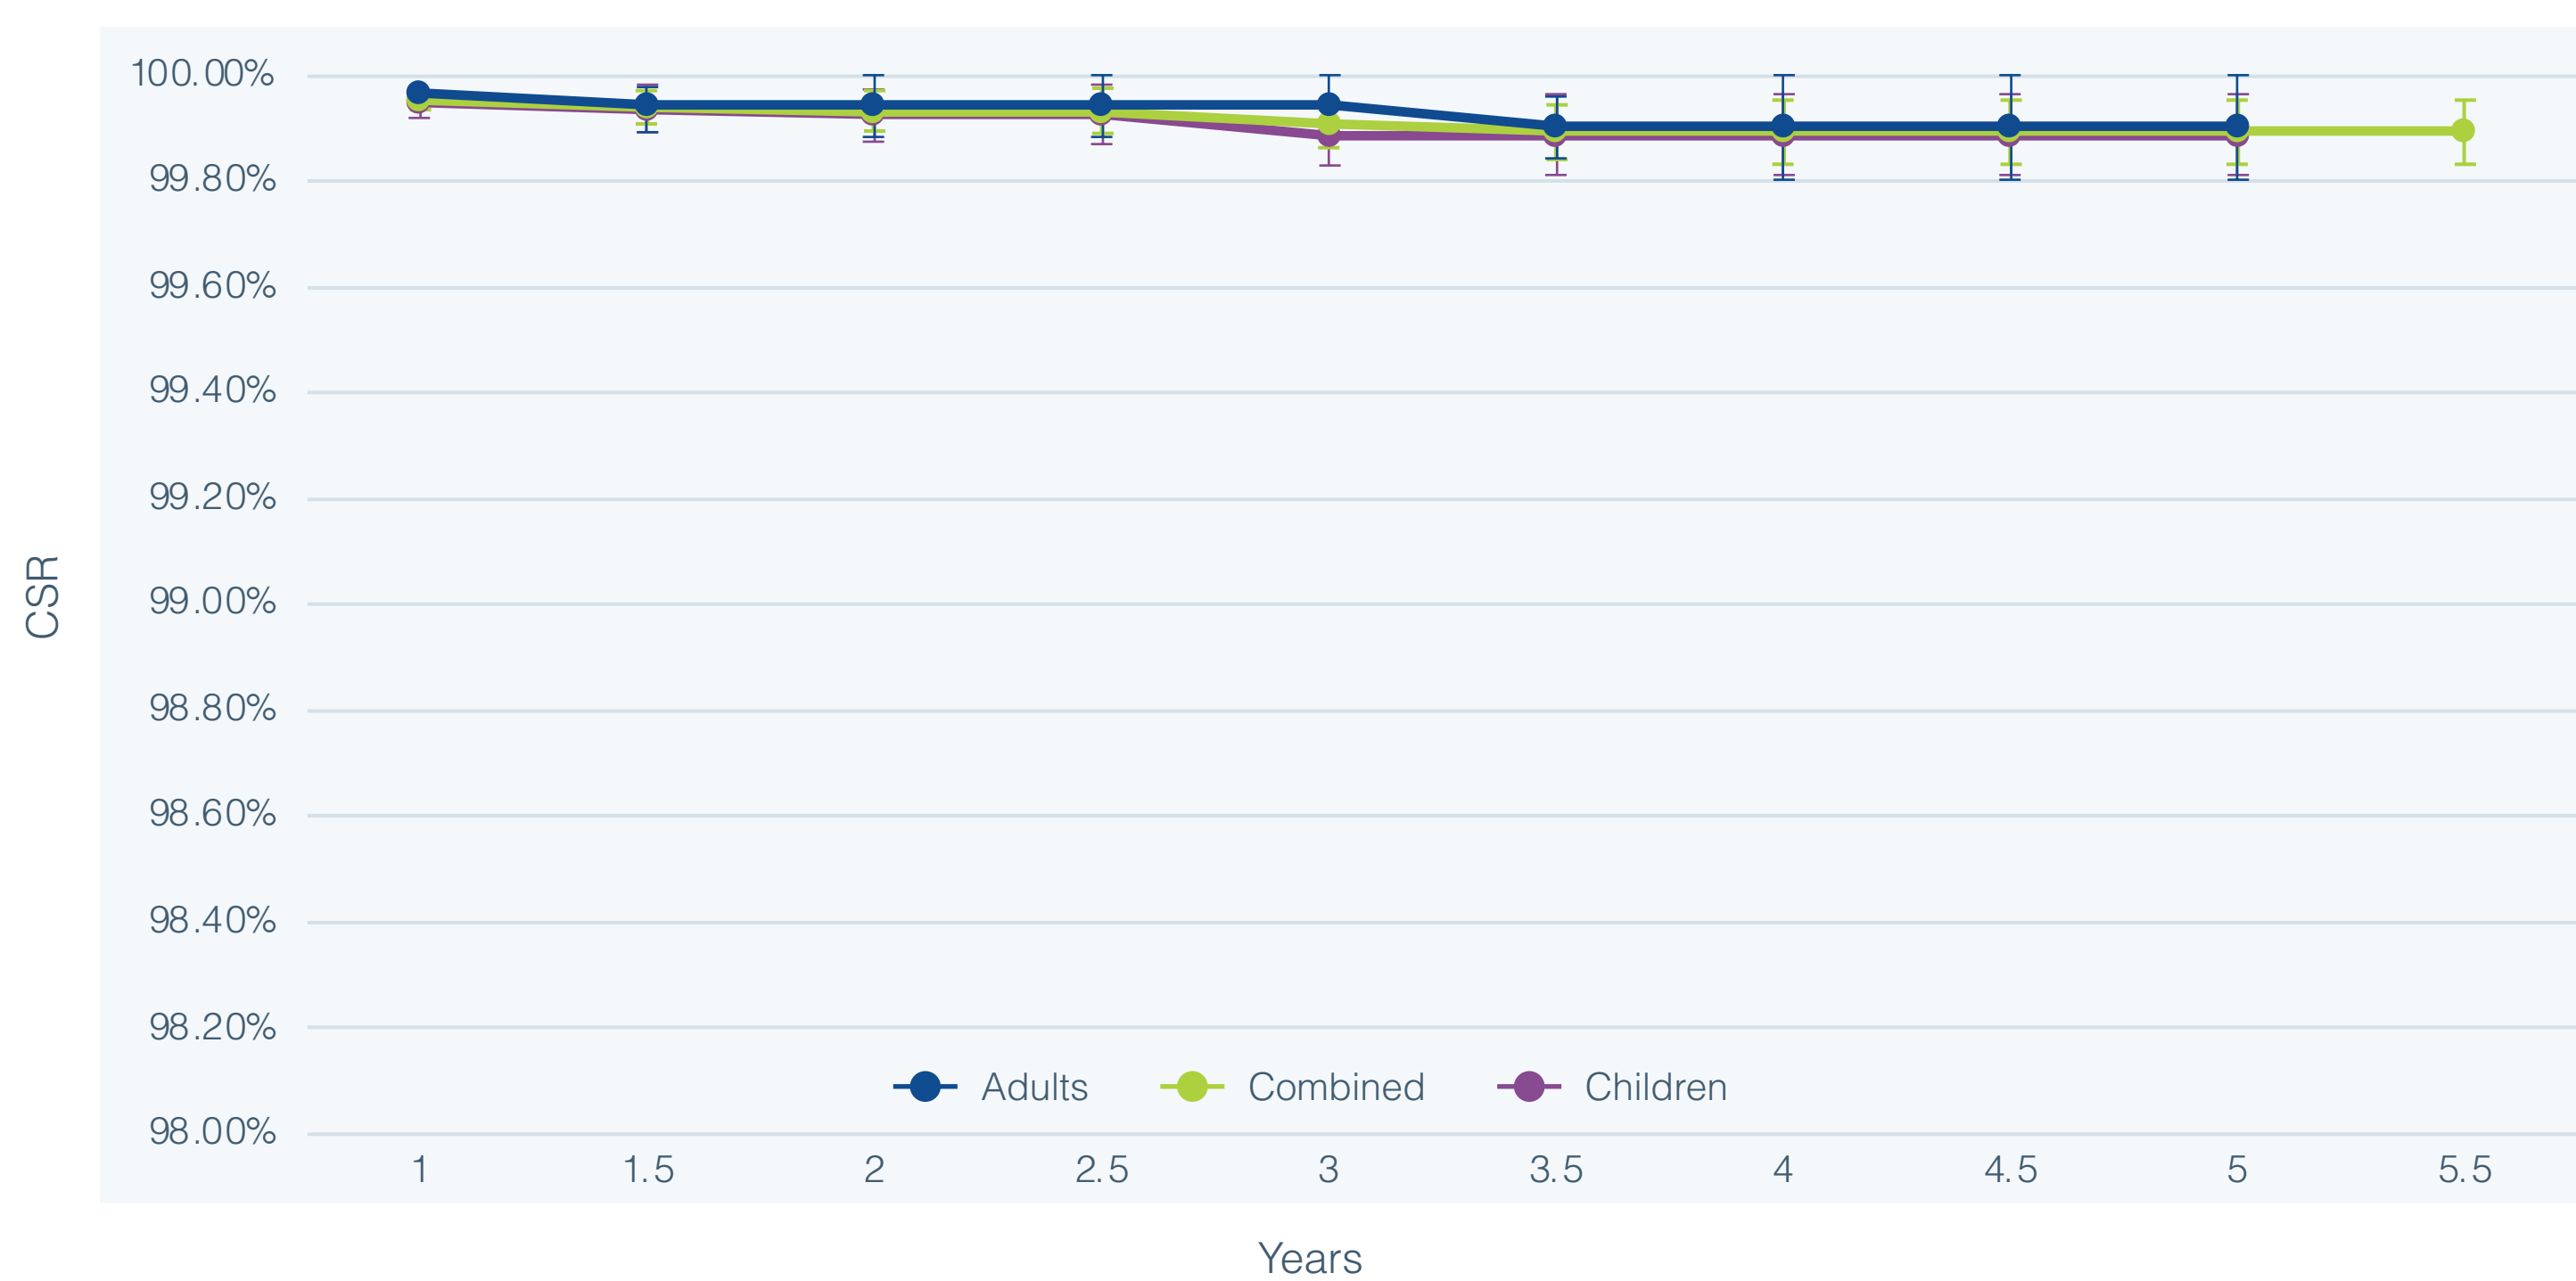

CUMULATIVE SURVIVAL RATE

Years in use	1	1.5	2	2.5	3	3.5	4	4.5	5	5.5
ADULTS	99.97%	99.95%	99.95%	99.95%	99.95%	99.91%	99.91%	99.91%	99.91%	N/A*
COMBINED	99.95%	99.94%	99.93%	99.93%	99.91%	99.89%	99.89%	99.89%	99.89%	99.89%
CHILDREN	99.95%	99.94%	99.92%	99.92%	99.89%	99.89%	99.89%	99.89%	99.89%	N/A*

*Sample size is not large enough for reporting.

ANSI/AAMI CI86

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

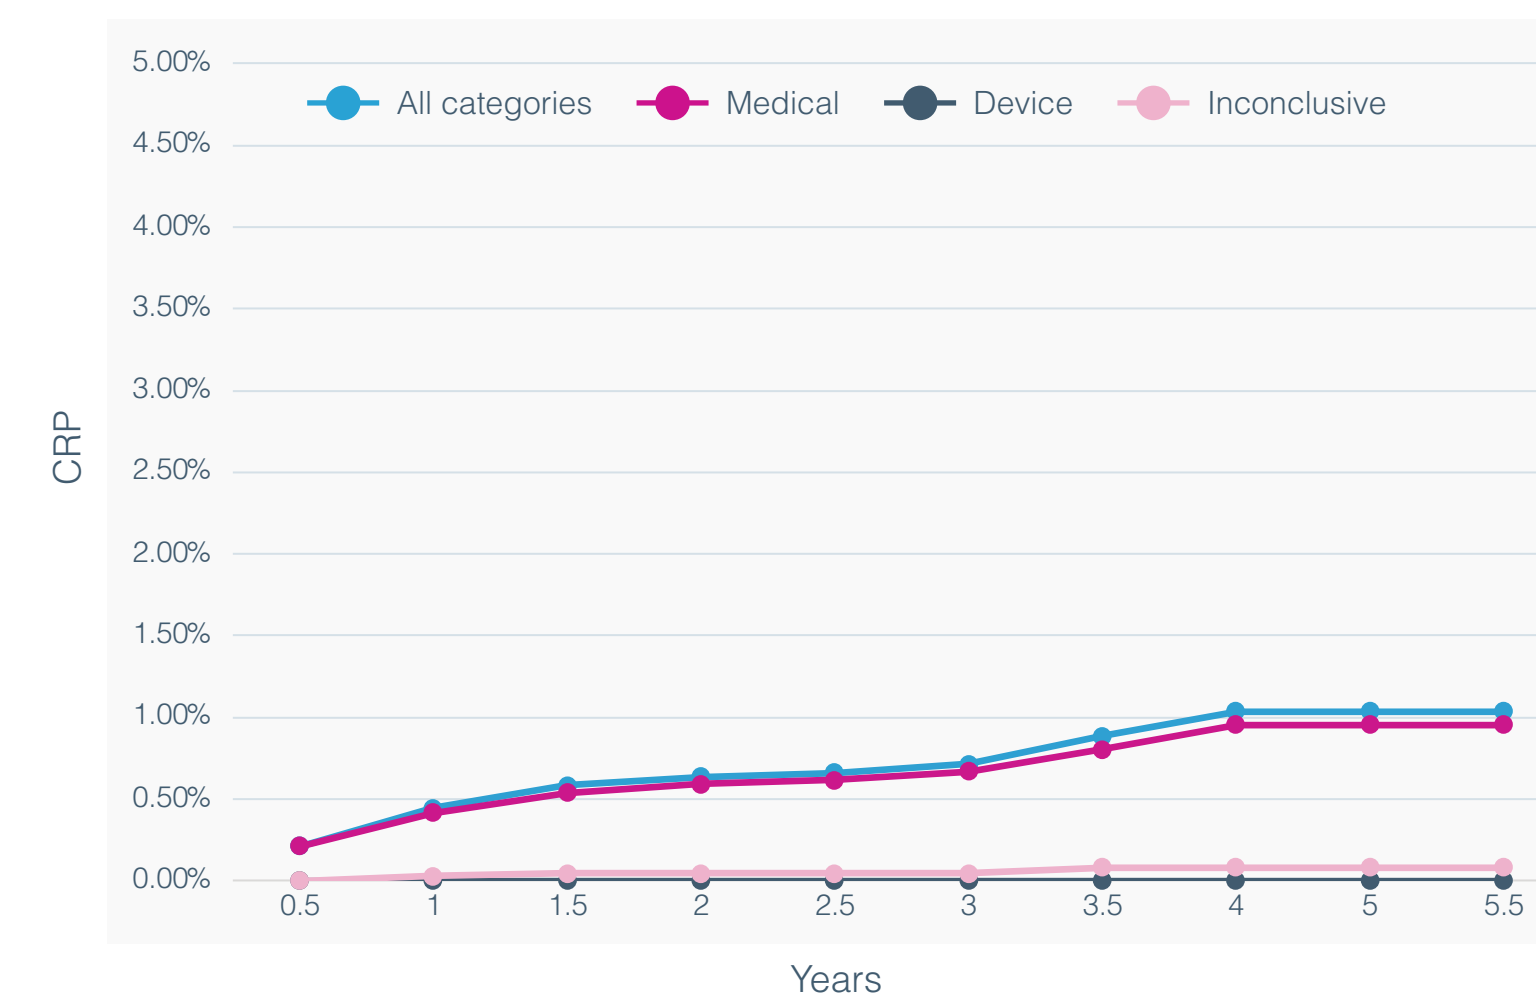

REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

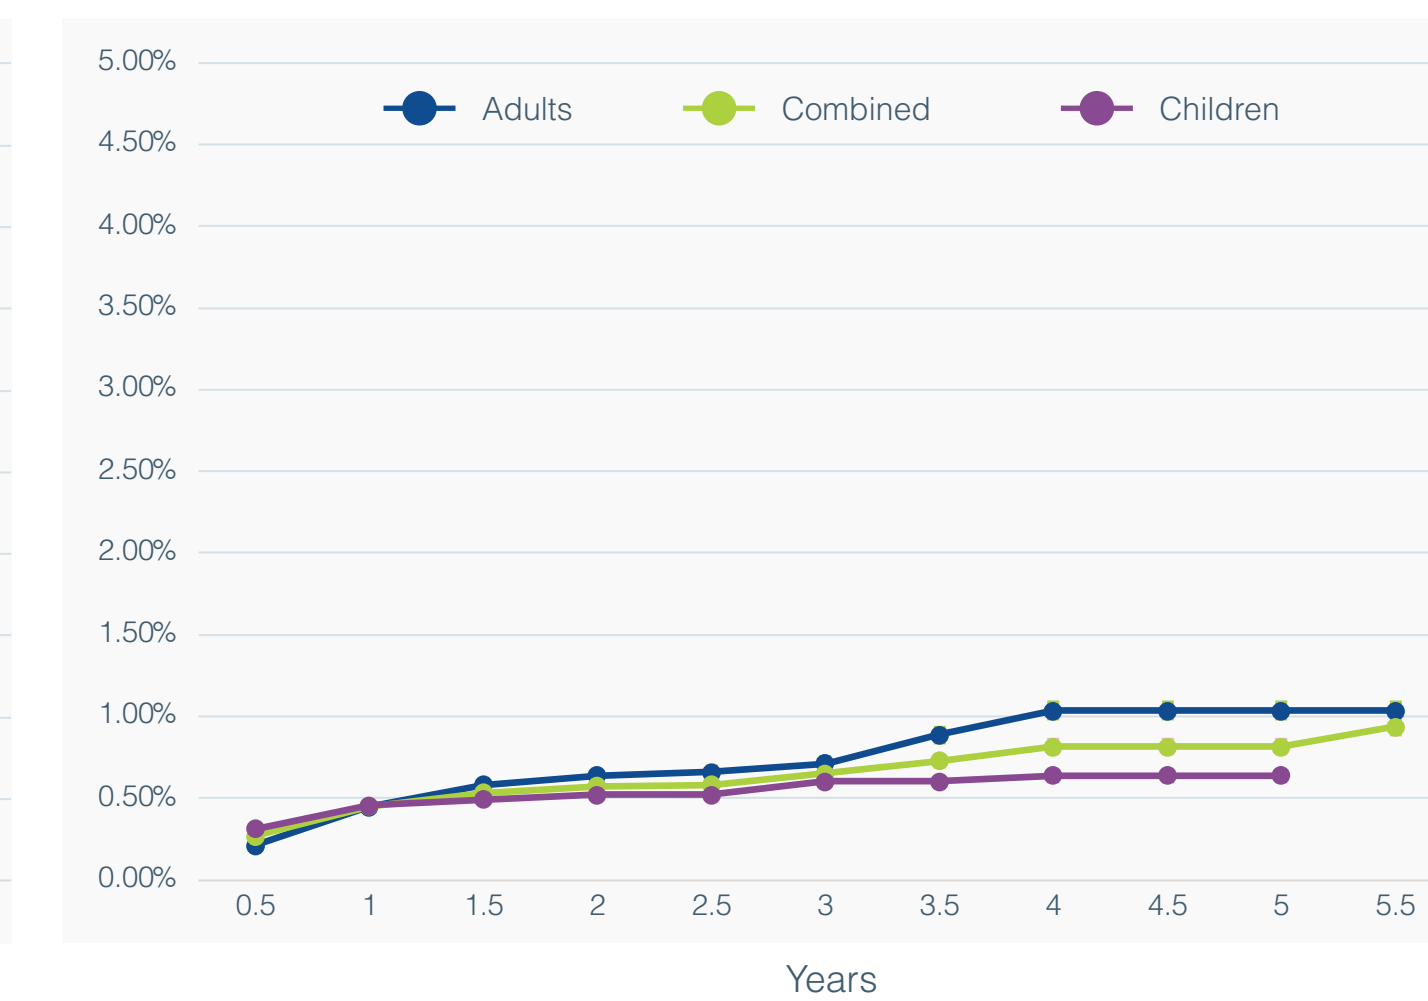

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

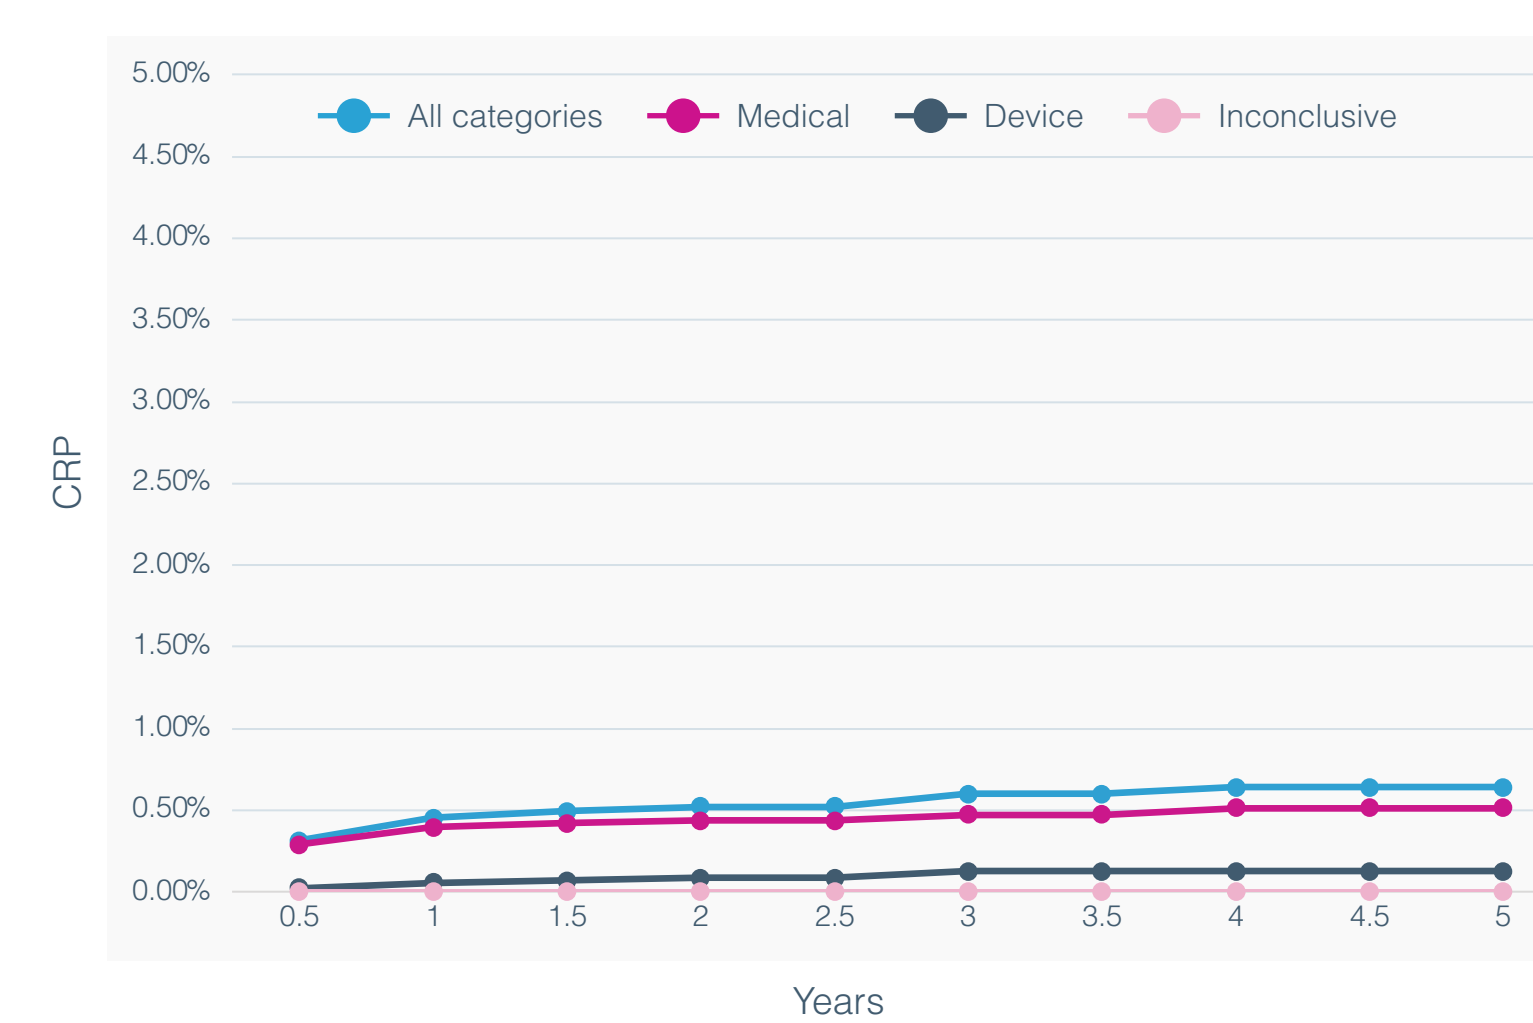

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

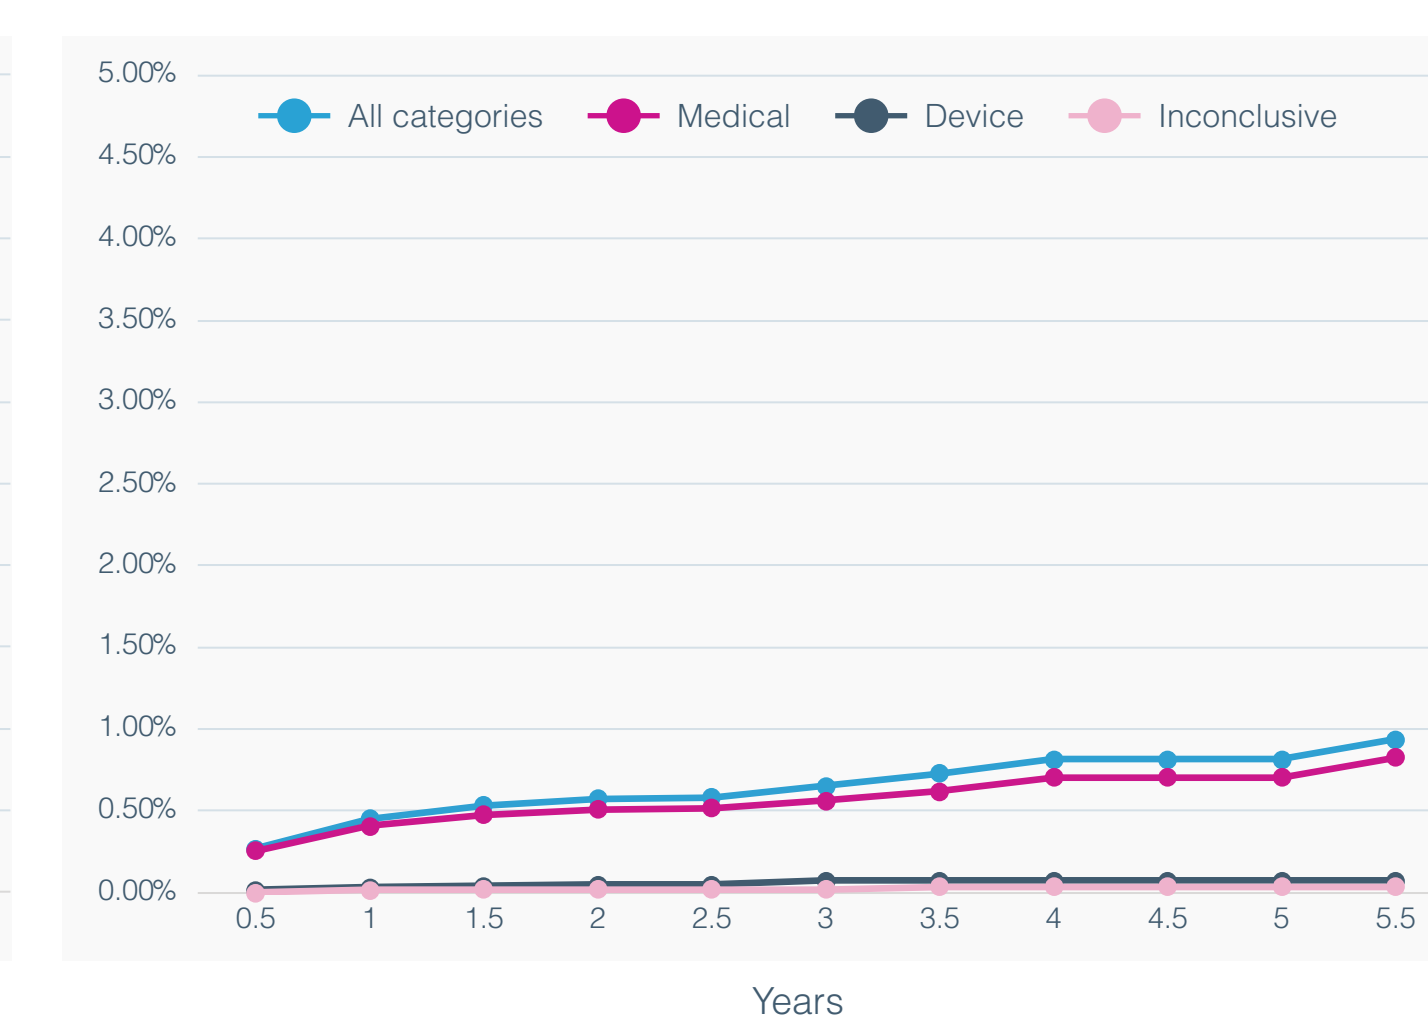

COMBINED ADULT AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	Total CI Lower
1	0.41%	0.03%	0.01%	0.45%	0.55%	0.35%
1.5	0.47%	0.04%	0.02%	0.53%	0.65%	0.42%
2	0.51%	0.05%	0.02%	0.57%	0.69%	0.45%
2.5	0.52%	0.05%	0.02%	0.58%	0.71%	0.46%
3	0.56%	0.07%	0.02%	0.65%	0.79%	0.52%
3.5	0.62%	0.07%	0.04%	0.73%	0.87%	0.58%
4	0.71%	0.07%	0.04%	0.81%	0.98%	0.64%
4.5	0.71%	0.07%	0.04%	0.81%	0.98%	0.64%
5	0.71%	0.07%	0.04%	0.81%	0.98%	0.64%
5.5	0.83%	0.07%	0.04%	0.93%	1.23%	0.64%

Please see the **Appendix** for a complete data set.

HIRES ULTRA 3D V1

The HiRes™ Ultra 3D (V1) cochlear implant is an update to the previous HiRes Ultra (V1) device. Advanced Bionics will continue to provide regular reliability updates on the HiRes Ultra platform as new data and information becomes available.

NUMBER OF REGISTERED HIRES ULTRA 3D (V1) IMPLANTS

As of April 1, 2026.
Last year of distribution: subject to voluntary field action February, 2020.[a]

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	4976	1729	6705[b]
ANSI/AAMI CI86	5253[c]	1452	6705

a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

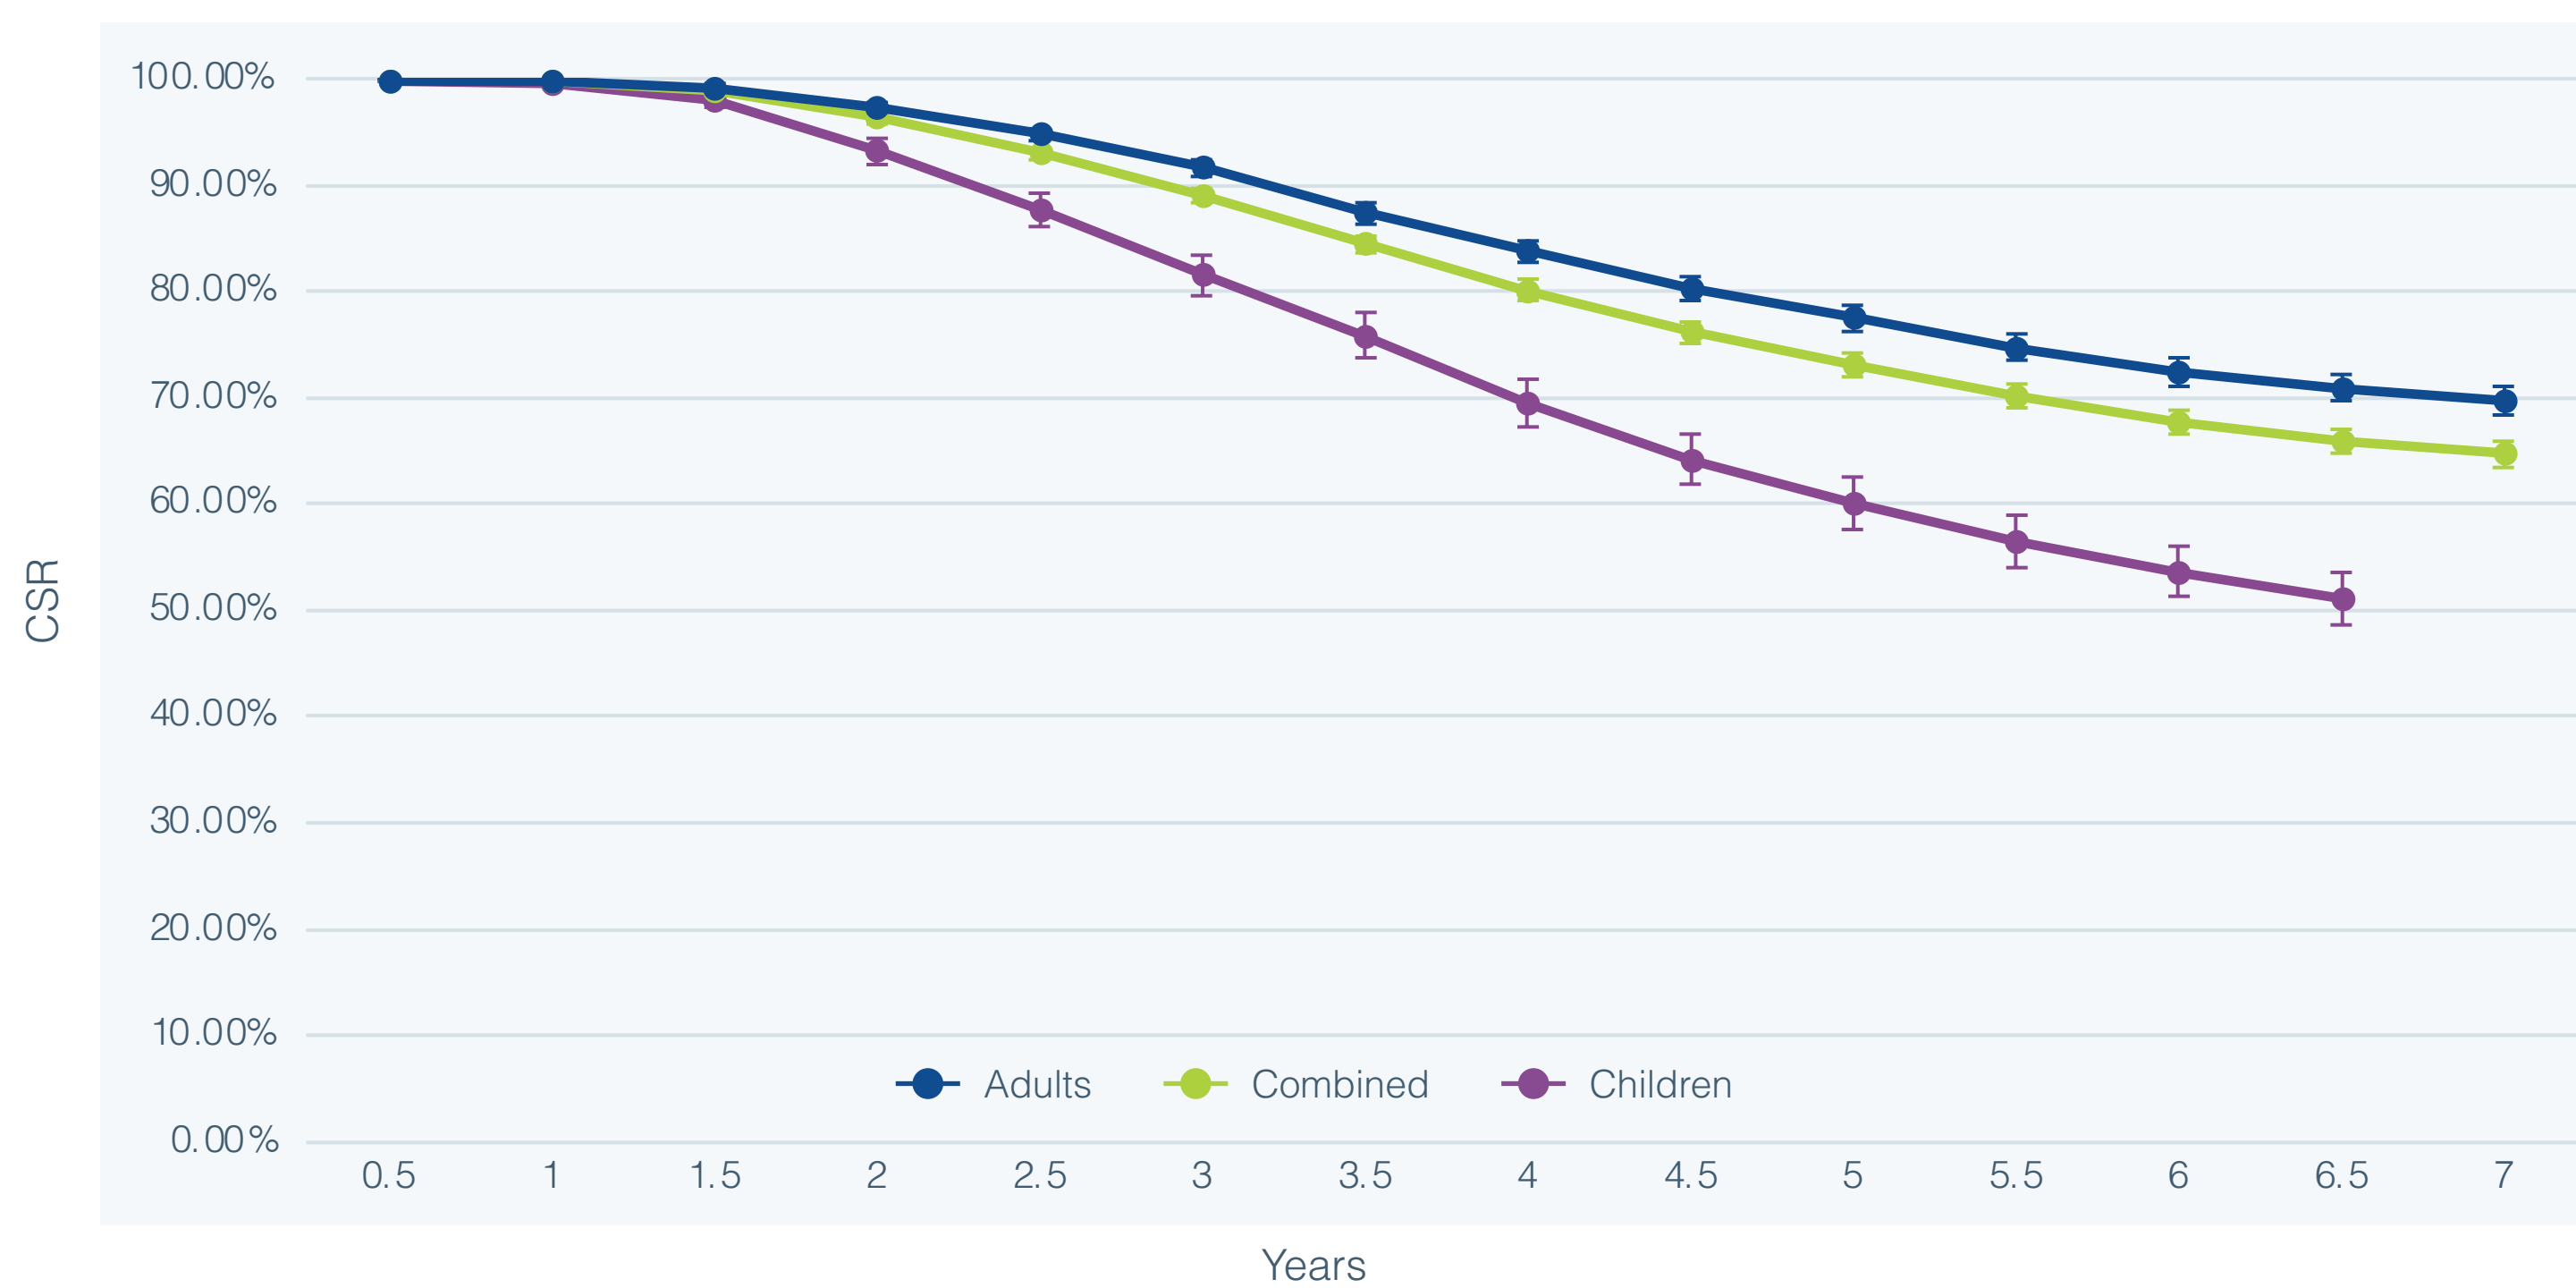

CUMULATIVE SURVIVAL RATE

Years in use	1	1.5	2	2.5	3	3.5	4	4.5	5	5.5	6	6.5	7
ADULTS	99.84%	99.27%	97.44%	94.82%	91.64%	87.40%	83.83%	80.33%	77.55%	74.76%	72.47%	70.96%	69.81%
COMBINED	99.77%	98.96%	96.35%	93.01%	89.06%	84.46%	80.15%	76.22%	73.10%	70.12%	67.70%	65.91%	64.71%
CHILDREN	99.59%	98.06%	93.21%	87.76%	81.55%	75.88%	69.43%	64.21%	60.07%	56.53%	53.67%	51.01%	N/A*

*Sample size is not large enough for reporting.

ANSI/AAMI CI86

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

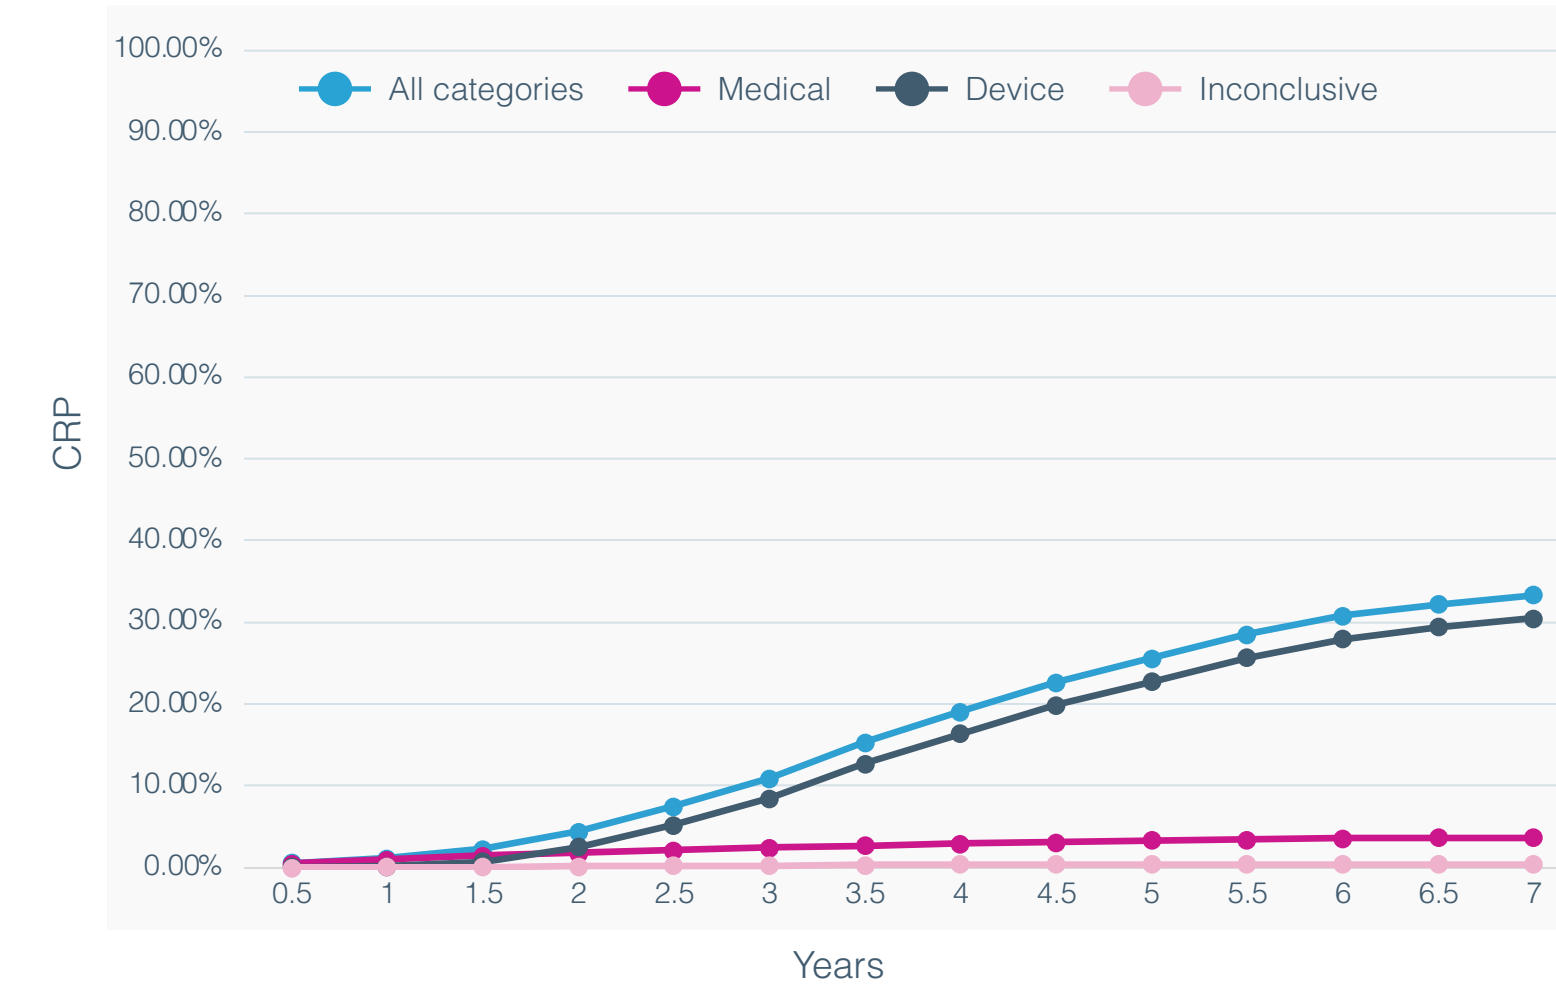

REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

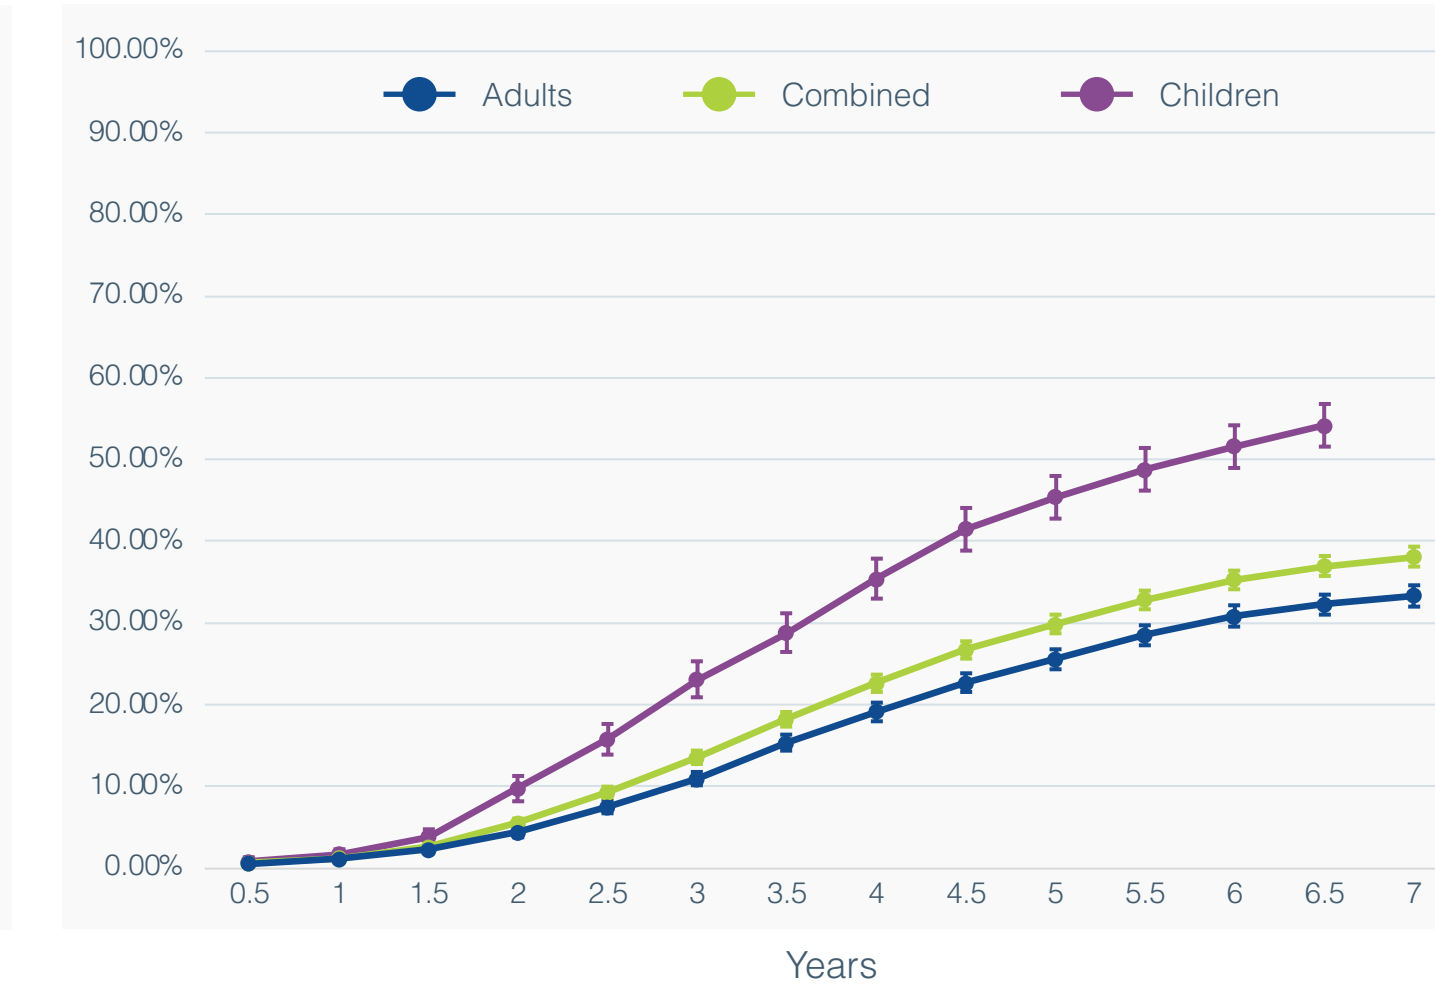

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

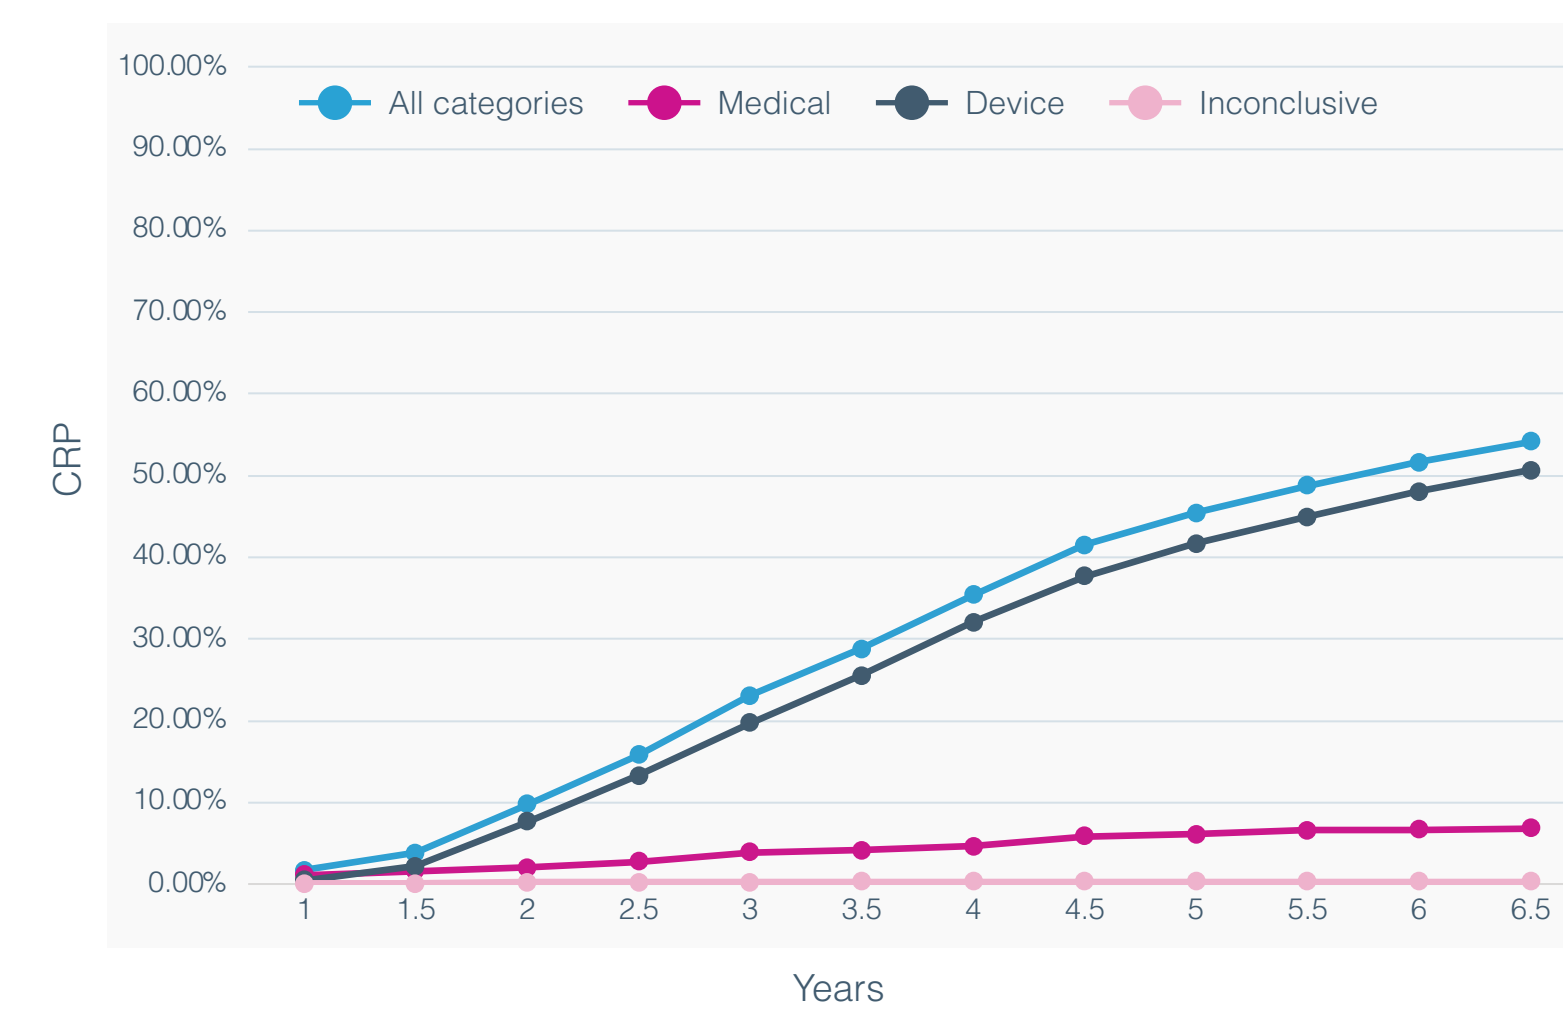

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

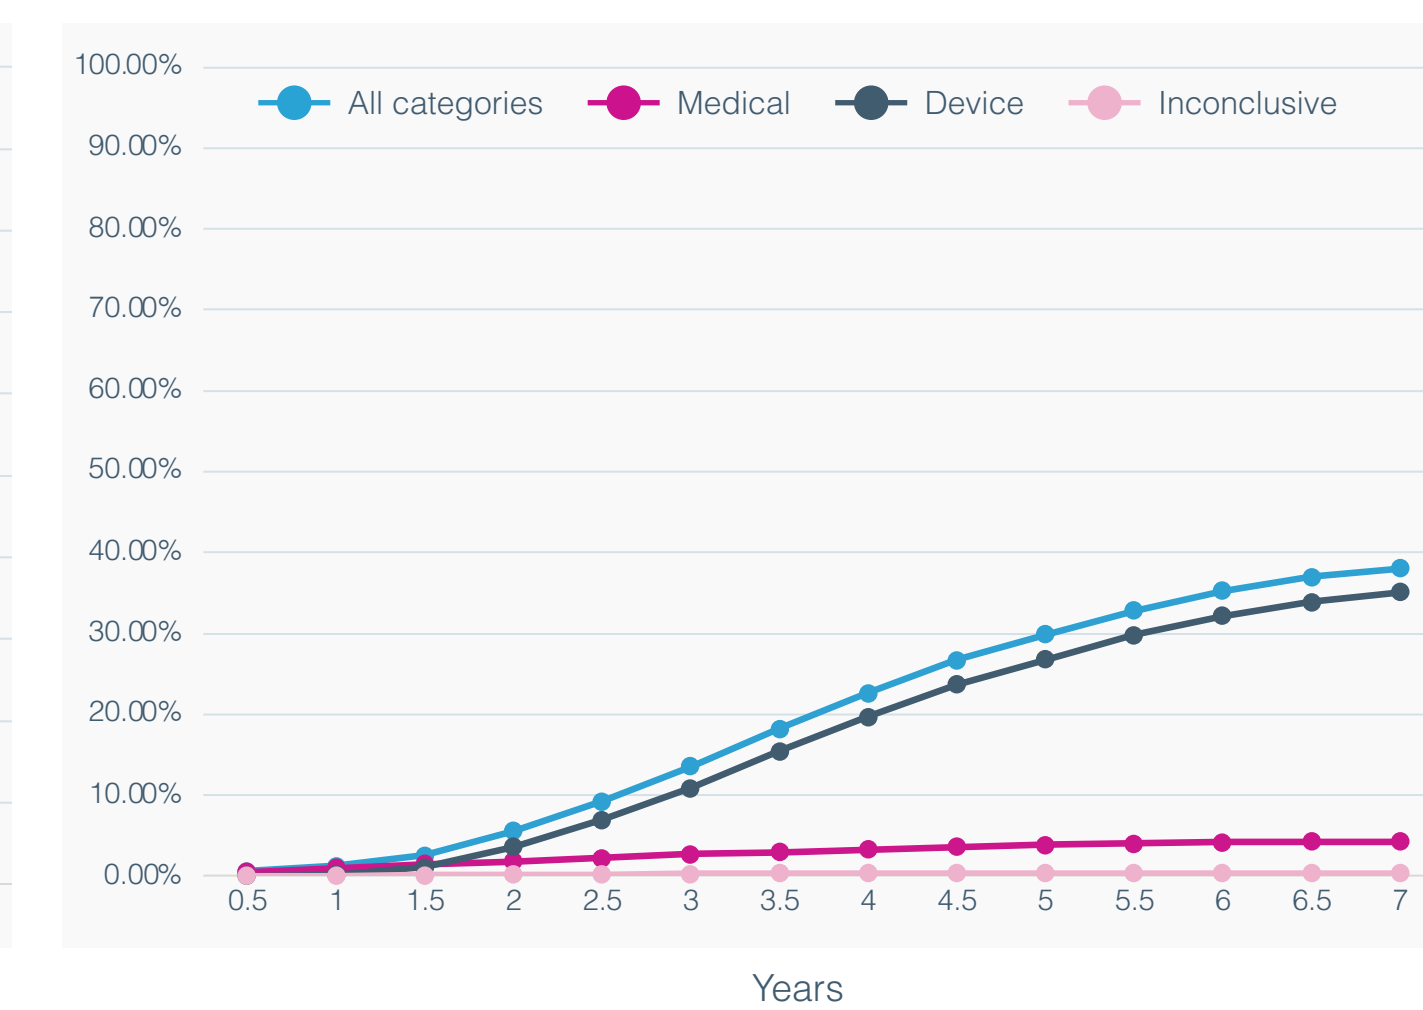

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	Total CI Lower
1	0.97%	0.23%	0.03%	1.22%	1.49%	0.96%
1.5	1.45%	1.06%	0.09%	2.58%	2.96%	2.20%
2	1.82%	3.60%	0.18%	5.53%	6.08%	4.98%
2.5	2.26%	6.95%	0.22%	9.26%	9.95%	8.56%
3	2.74%	10.91%	0.23%	13.55%	14.37%	12.73%
3.5	2.99%	15.45%	0.32%	18.24%	19.17%	17.31%
4	3.25%	19.72%	0.36%	22.61%	23.62%	21.61%
4.5	3.60%	23.68%	0.36%	26.70%	27.76%	25.63%
5	3.83%	26.77%	0.38%	29.85%	30.95%	28.74%
5.5	4.00%	29.77%	0.38%	32.84%	33.98%	31.71%
6	4.18%	32.20%	0.38%	35.29%	36.45%	34.13%
6.5	4.23%	33.90%	0.38%	36.94%	38.11%	35.77%
7	4.27%	35.07%	0.38%	38.08%	39.28%	36.87%

Please see the **Appendix** for a complete data set.

HIRES ULTRA V1

The HiRes™ Ultra (V1) cochlear implant was subject to a Voluntary Field Action initiated by Advanced Bionics in February 2020, and was withdrawn from sale worldwide. This was due to recognition of a common failure mode for a small number of devices, resulting in loss of clinical benefit. Advanced Bionics will continue to provide regular reliability updates on the HiRes Ultra platform as new data and information becomes available.

NUMBER OF REGISTERED HIRES ULTRA (V1) IMPLANTS

As of April 1, 2026.
Last year of distribution: subject to voluntary field action February, 2020.[a]

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	8006	4558	12564[b]
ANSI/AAMI CI86	8567[c]	3997	12564

a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

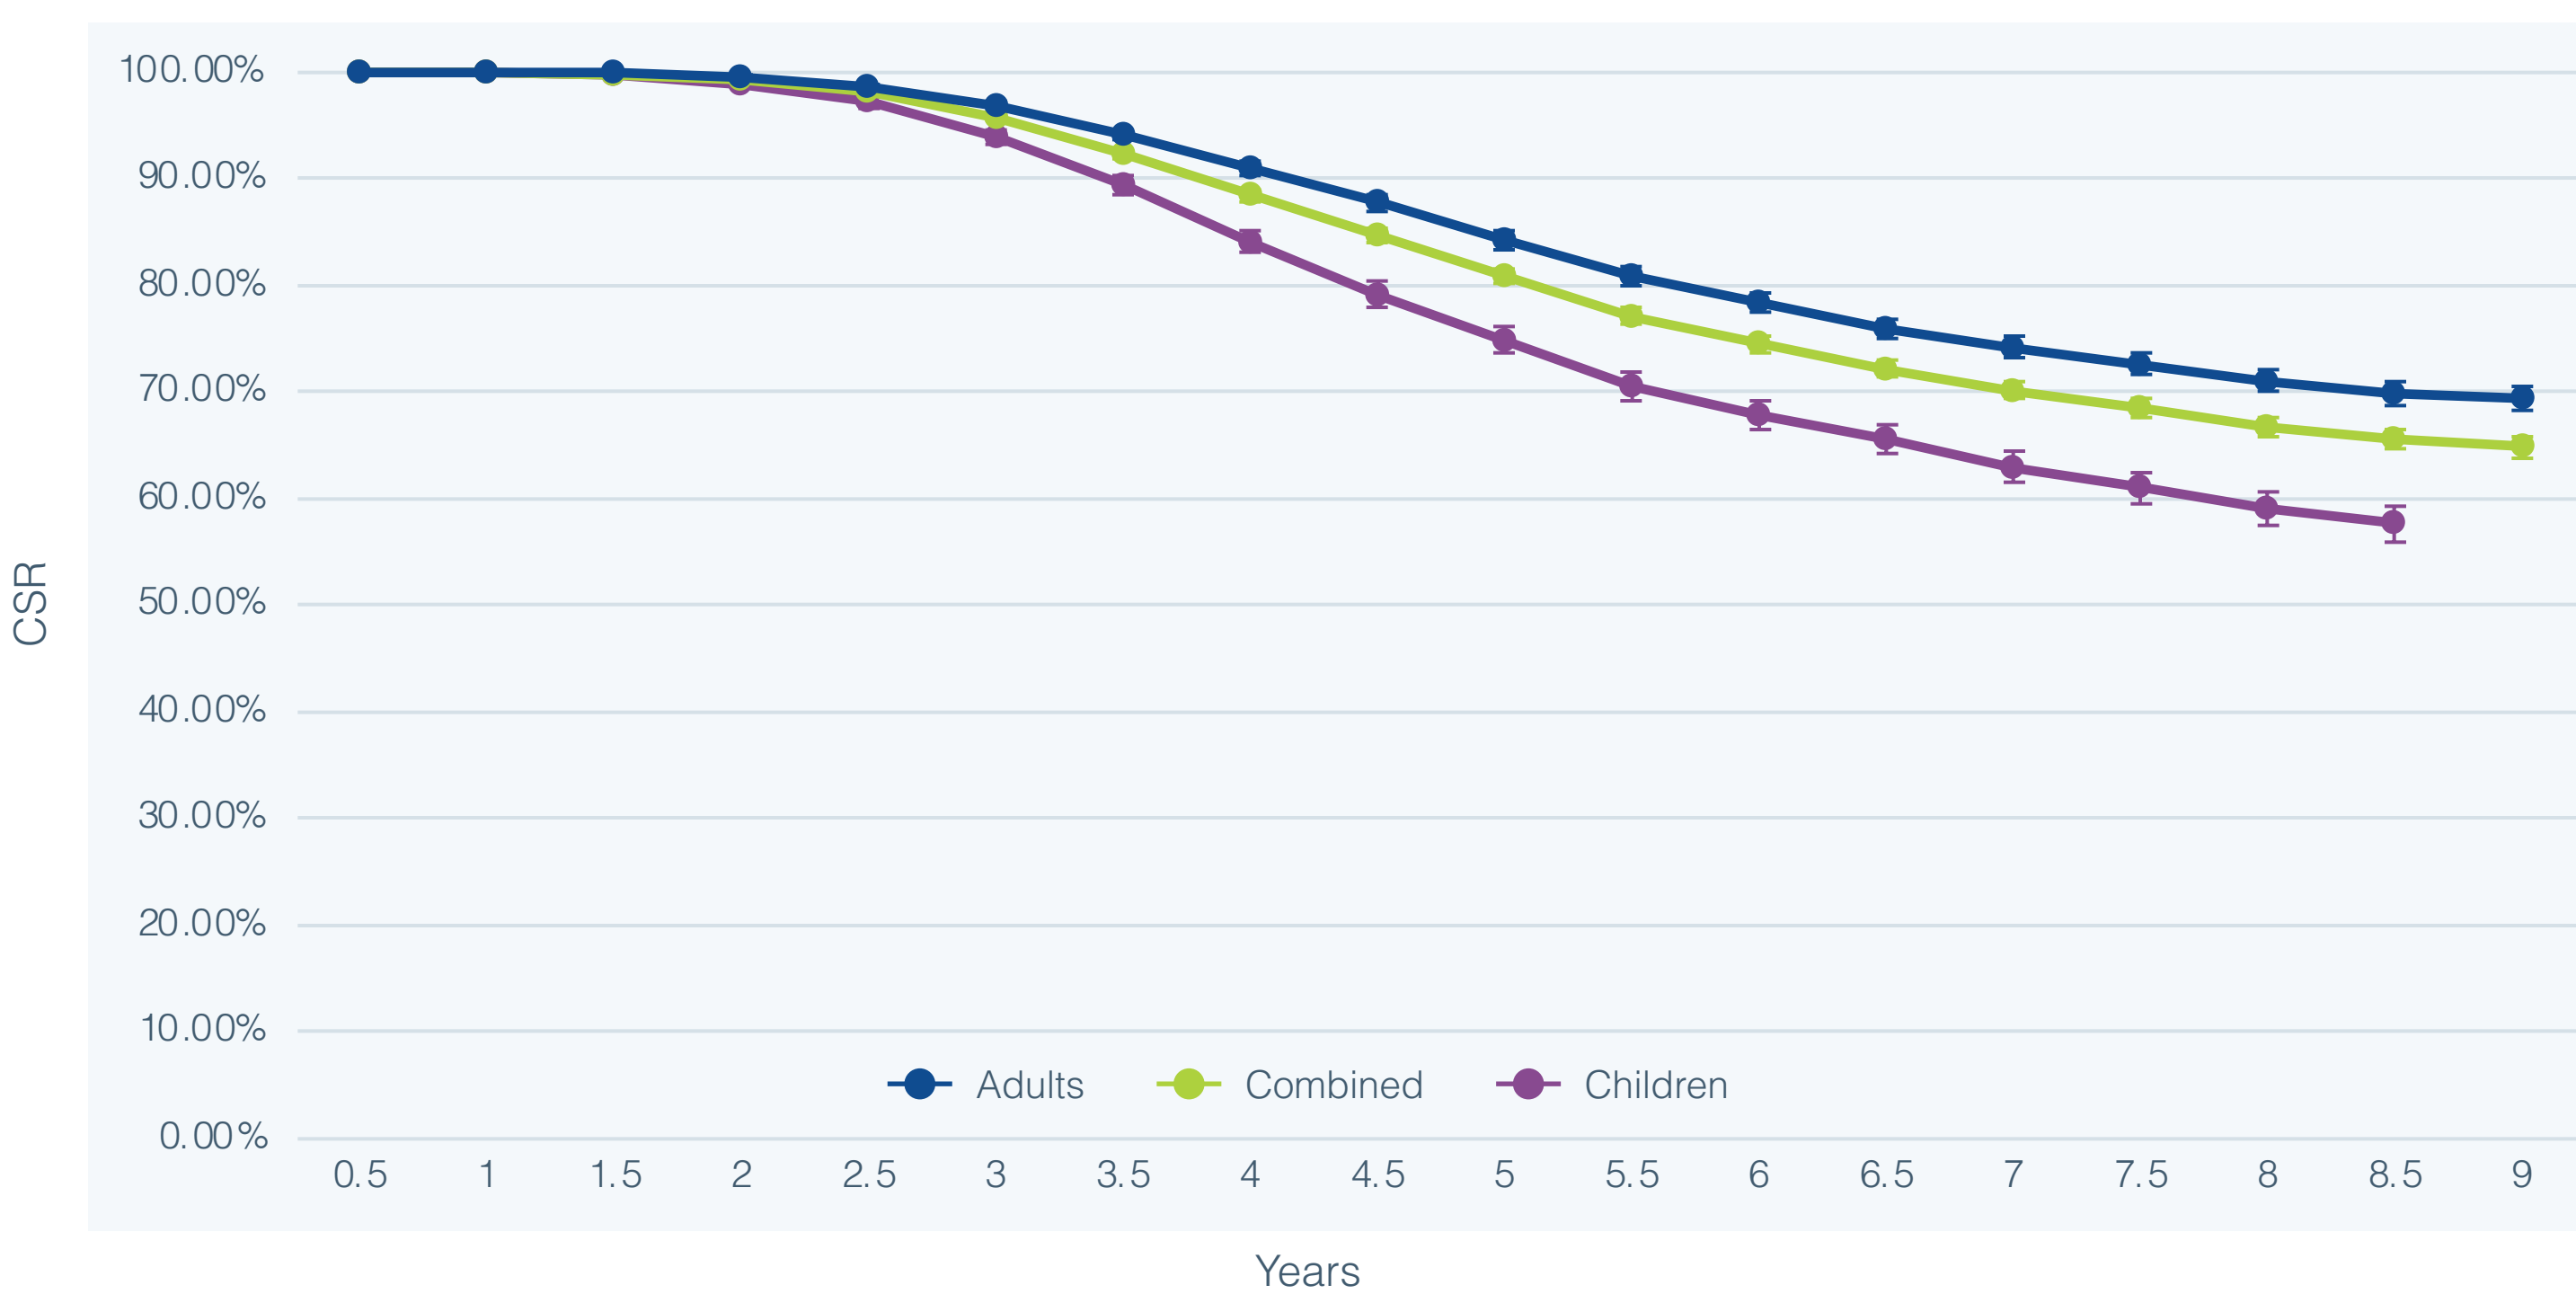

CUMULATIVE SURVIVAL RATE

Years in use	1	1.5	2	2.5	3	3.5	4	4.5	5	5.5	6	6.5	7	7.5	8	8.5	9
ADULTS	99.98%	99.90%	99.53%	98.59%	96.78%	94.08%	90.93%	87.71%	84.17%	80.90%	78.34%	75.90%	74.18%	72.59%	71.00%	69.85%	69.28%
COMBINED	99.94%	99.78%	99.27%	98.05%	95.71%	92.35%	88.41%	84.57%	80.75%	77.07%	74.51%	72.14%	70.11%	68.44%	66.76%	65.58%	64.84%
CHILDREN	99.89%	99.58%	98.83%	97.10%	93.85%	89.34%	84.04%	79.09%	74.80%	70.41%	67.83%	65.59%	62.87%	60.95%	58.98%	57.65%	N/A*

*Sample size is not large enough for reporting.

ANSI/AAMI CI86

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

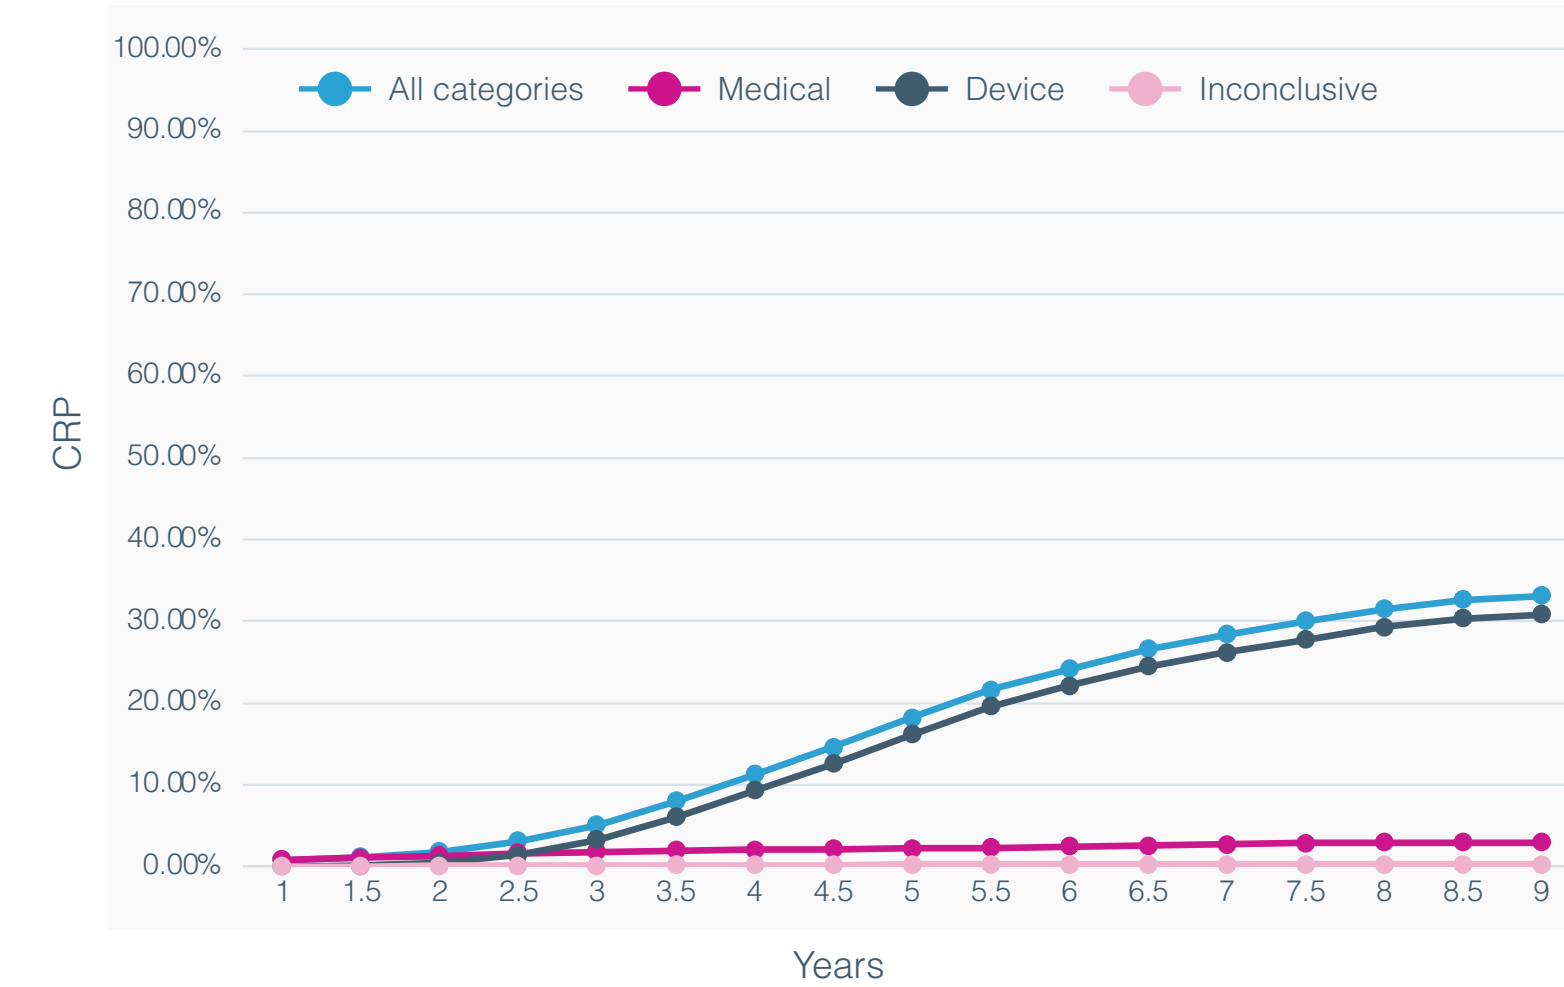

REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

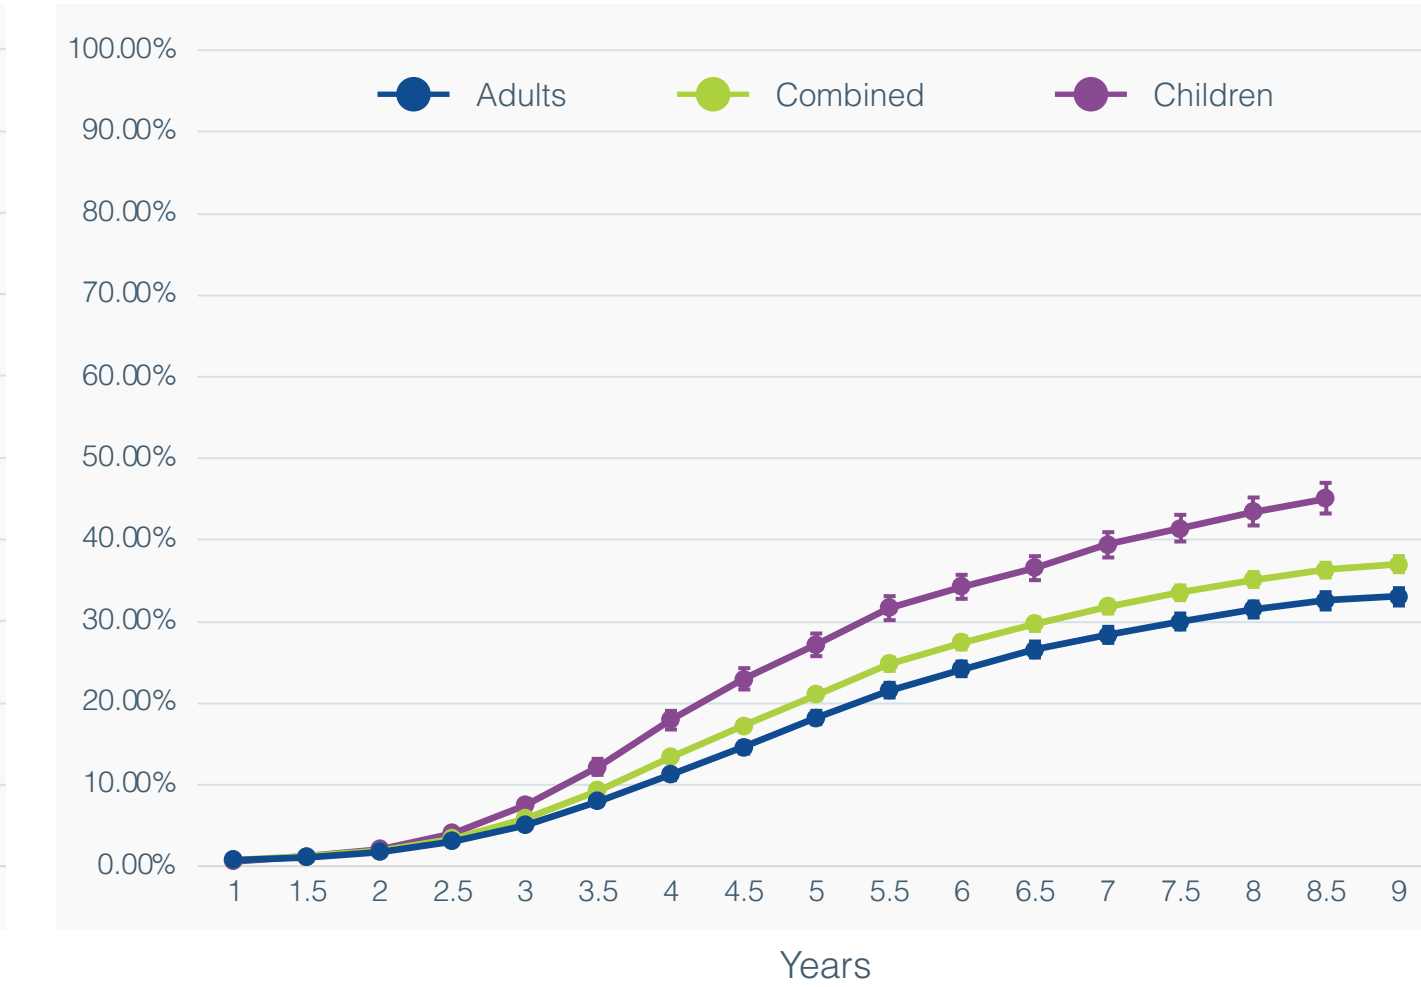

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

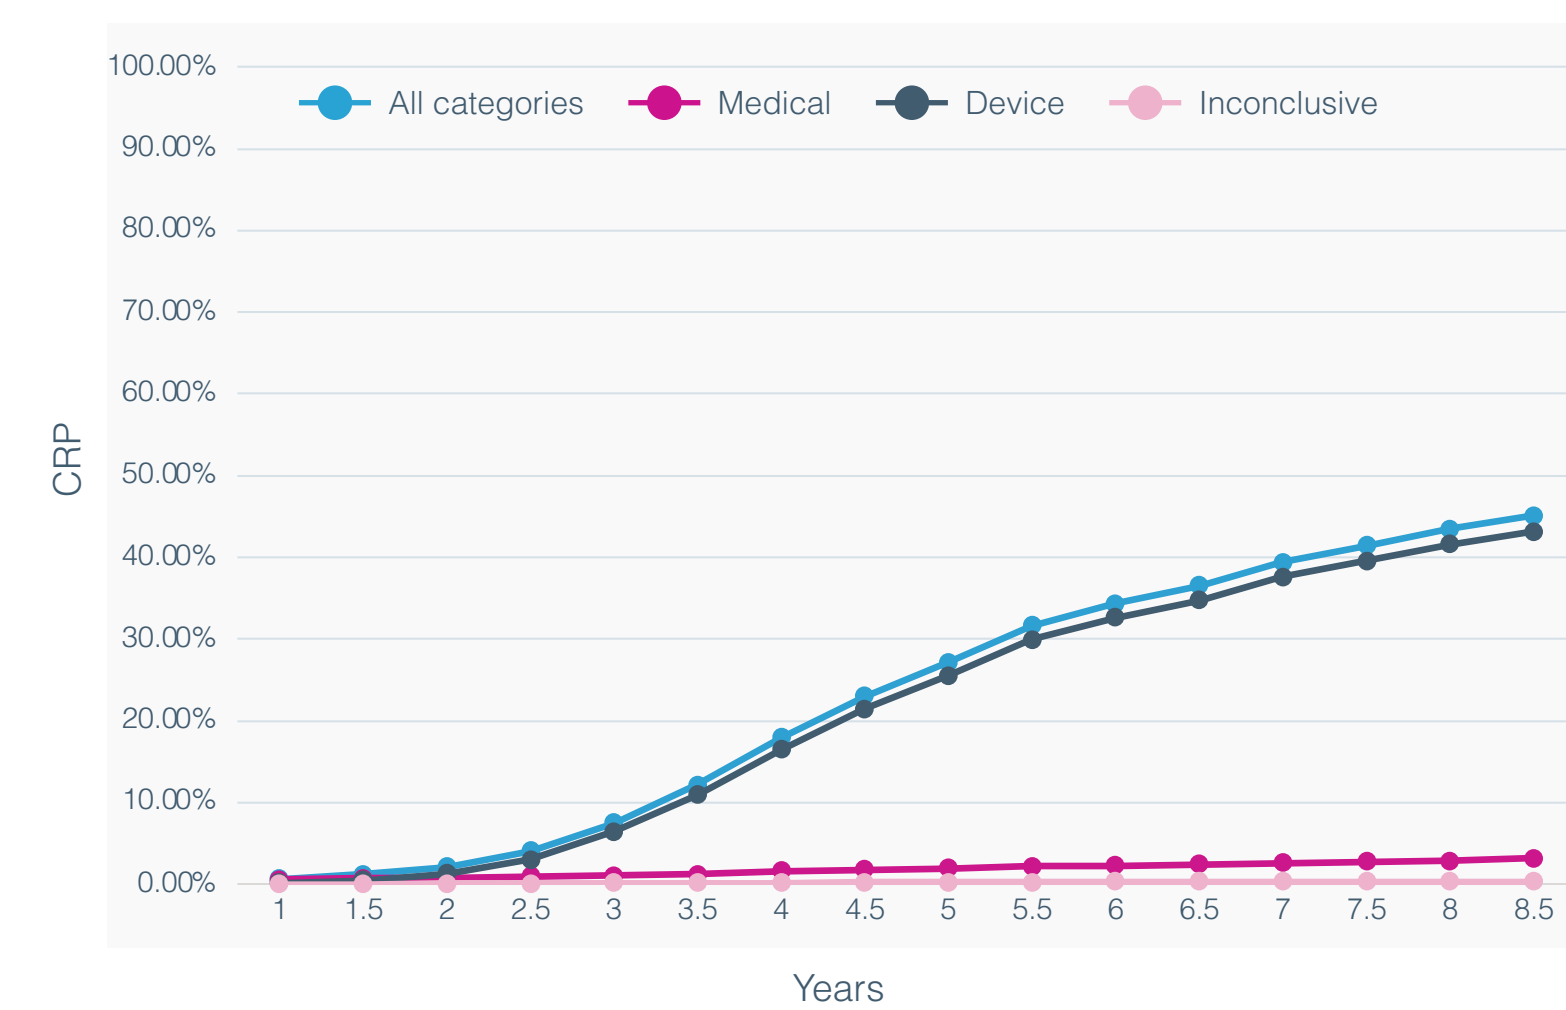

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

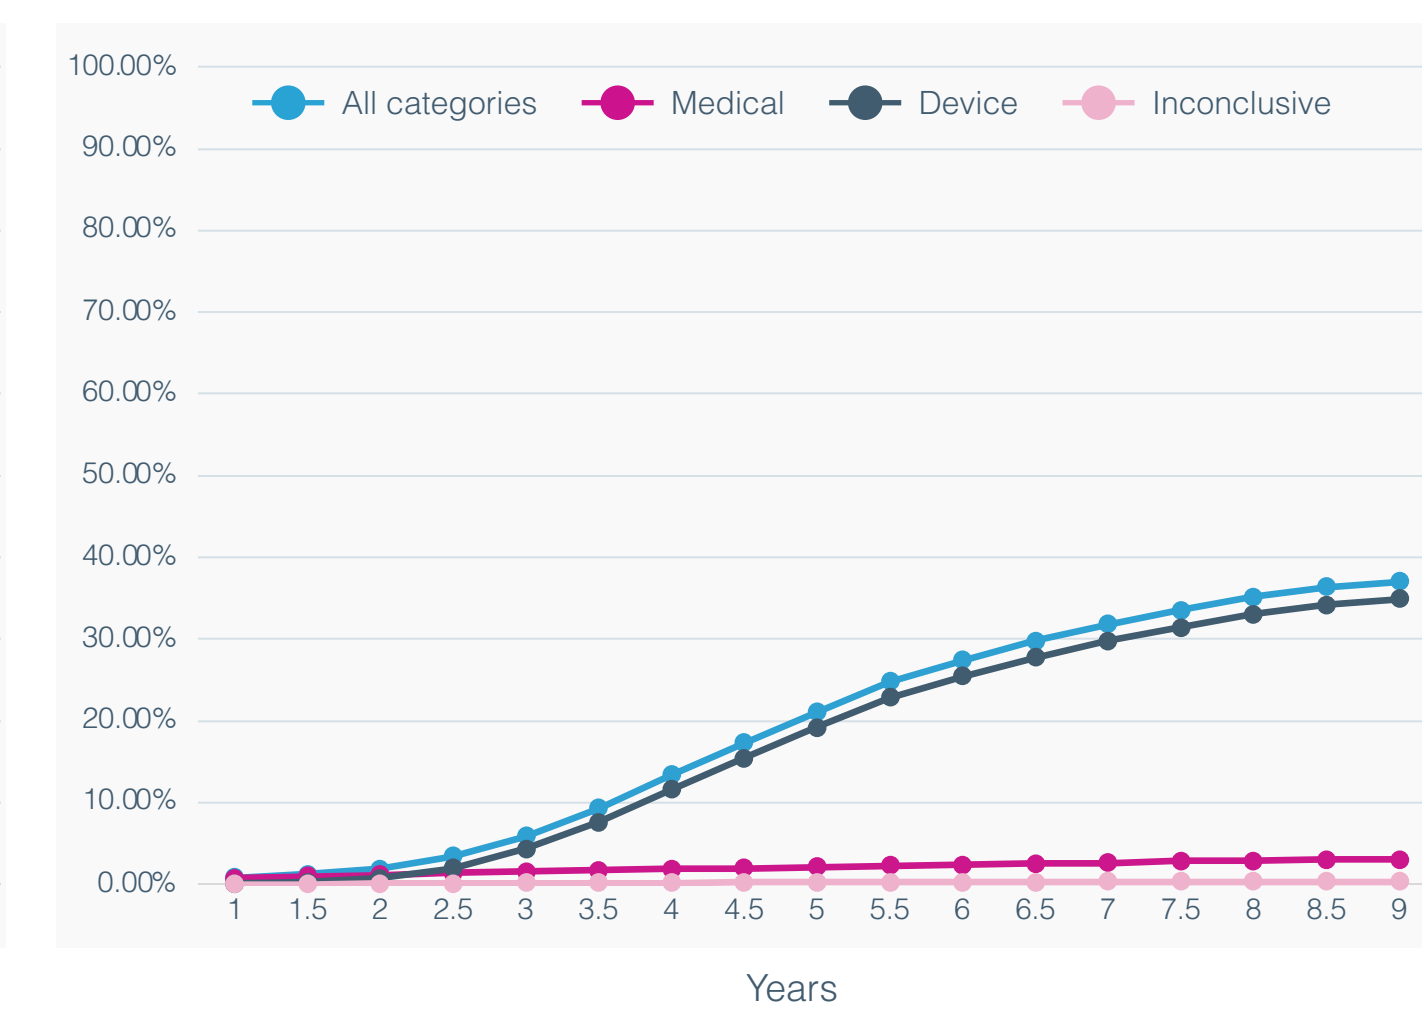

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	Total CI Lower
1	0.71%	0.06%	0.02%	0.78%	0.93%	0.63%
1.5	0.93%	0.22%	0.02%	1.17%	1.36%	0.98%
2	1.15%	0.71%	0.05%	1.90%	2.14%	1.66%
2.5	1.39%	1.93%	0.08%	3.37%	3.69%	3.06%
3	1.54%	4.28%	0.11%	5.86%	6.27%	5.45%
3.5	1.69%	7.61%	0.15%	9.32%	9.82%	8.81%
4	1.87%	11.58%	0.16%	13.37%	13.97%	12.77%
4.5	1.98%	15.42%	0.20%	17.25%	17.91%	16.59%
5	2.10%	19.18%	0.22%	21.05%	21.77%	20.33%
5.5	2.26%	22.87%	0.24%	24.79%	25.55%	24.03%
6	2.39%	25.43%	0.26%	27.40%	28.19%	26.62%
6.5	2.49%	27.75%	0.27%	29.75%	30.55%	28.94%
7	2.63%	29.78%	0.28%	31.82%	32.65%	30.99%
7.5	2.81%	31.41%	0.28%	33.53%	34.39%	32.68%
8	2.85%	33.06%	0.28%	35.15%	36.03%	34.27%
8.5	2.98%	34.21%	0.28%	36.35%	37.27%	35.43%
9	2.98%	34.87%	0.28%	36.99%	37.95%	36.03%

Please see the **Appendix** for a complete data set.

HIRES 90K ADVANTAGE

The HiRes 90K™ Advantage cochlear implant offers mechanical improvements over its predecessor, the HiRes 90K cochlear implant. It has the capability to offer advanced sound coding strategies, together with the security of a deep bone bed.

NUMBER OF REGISTERED HIRES 90K ADVANTAGE IMPLANTS

As of April 1, 2026.
Last year of distribution: 2023.[a]

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	18504	24723	43227[b]
ANSI/AAMI CI86	21115[c]	22112	43227

a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

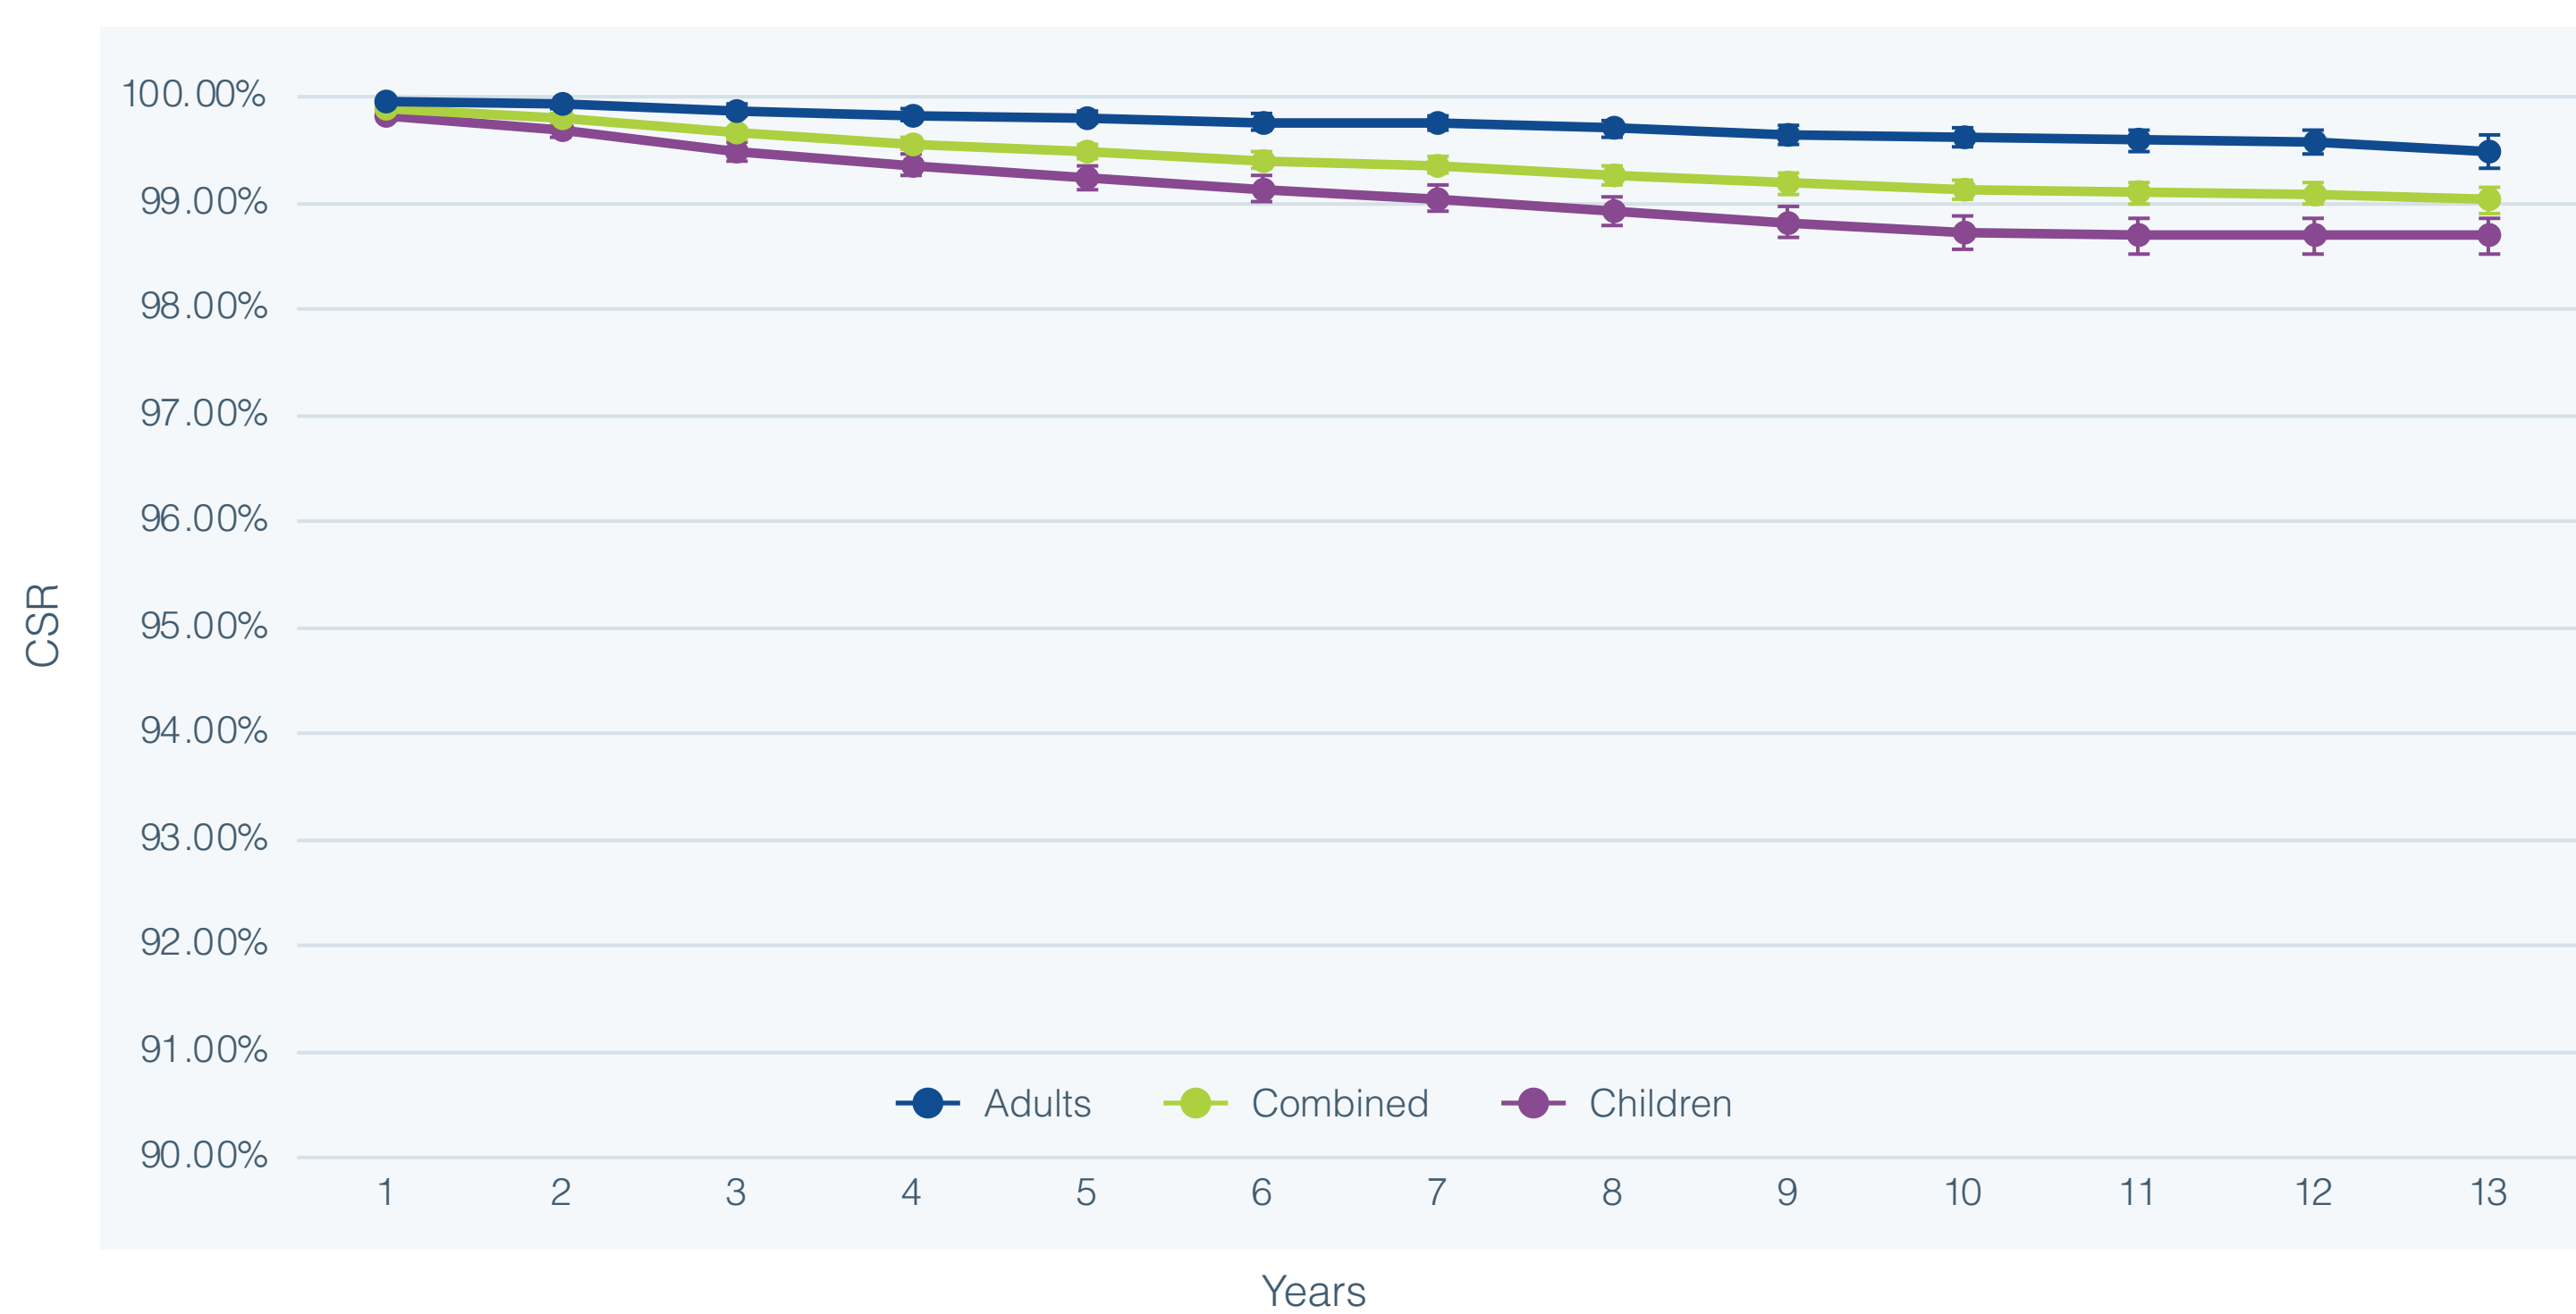

CUMULATIVE SURVIVAL RATE

Years in use	1	2	3	4	5	6	7	8	9	10	11	12	13
ADULTS	99.95%	99.92%	99.87%	99.83%	99.81%	99.76%	99.75%	99.70%	99.64%	99.62%	99.59%	99.57%	99.48%
COMBINED	99.88%	99.79%	99.66%	99.56%	99.48%	99.40%	99.35%	99.26%	99.18%	99.13%	99.10%	99.08%	99.03%
CHILDREN	99.83%	99.69%	99.49%	99.36%	99.23%	99.13%	99.04%	98.92%	98.81%	98.73%	98.69%	98.69%	98.69%

ANSI/AAMI CI86

REMOVAL RATES ANALYSIS CATEGORIES
FOR ADULTS

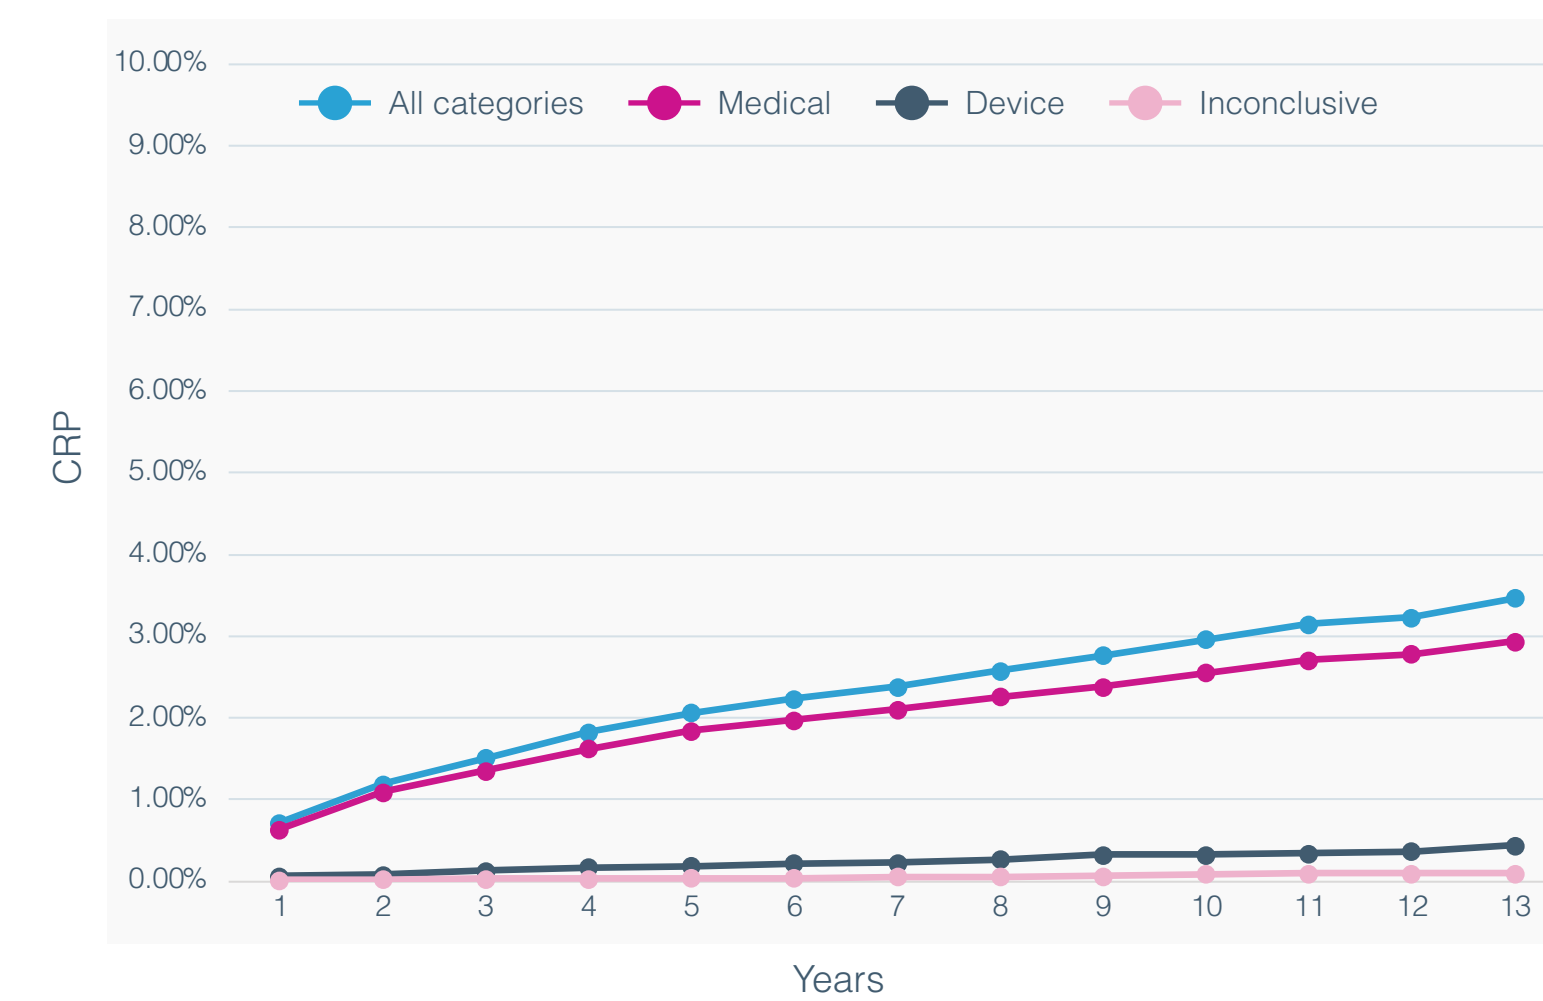

REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES
AND DIFFERENT PATIENTS POPULATION

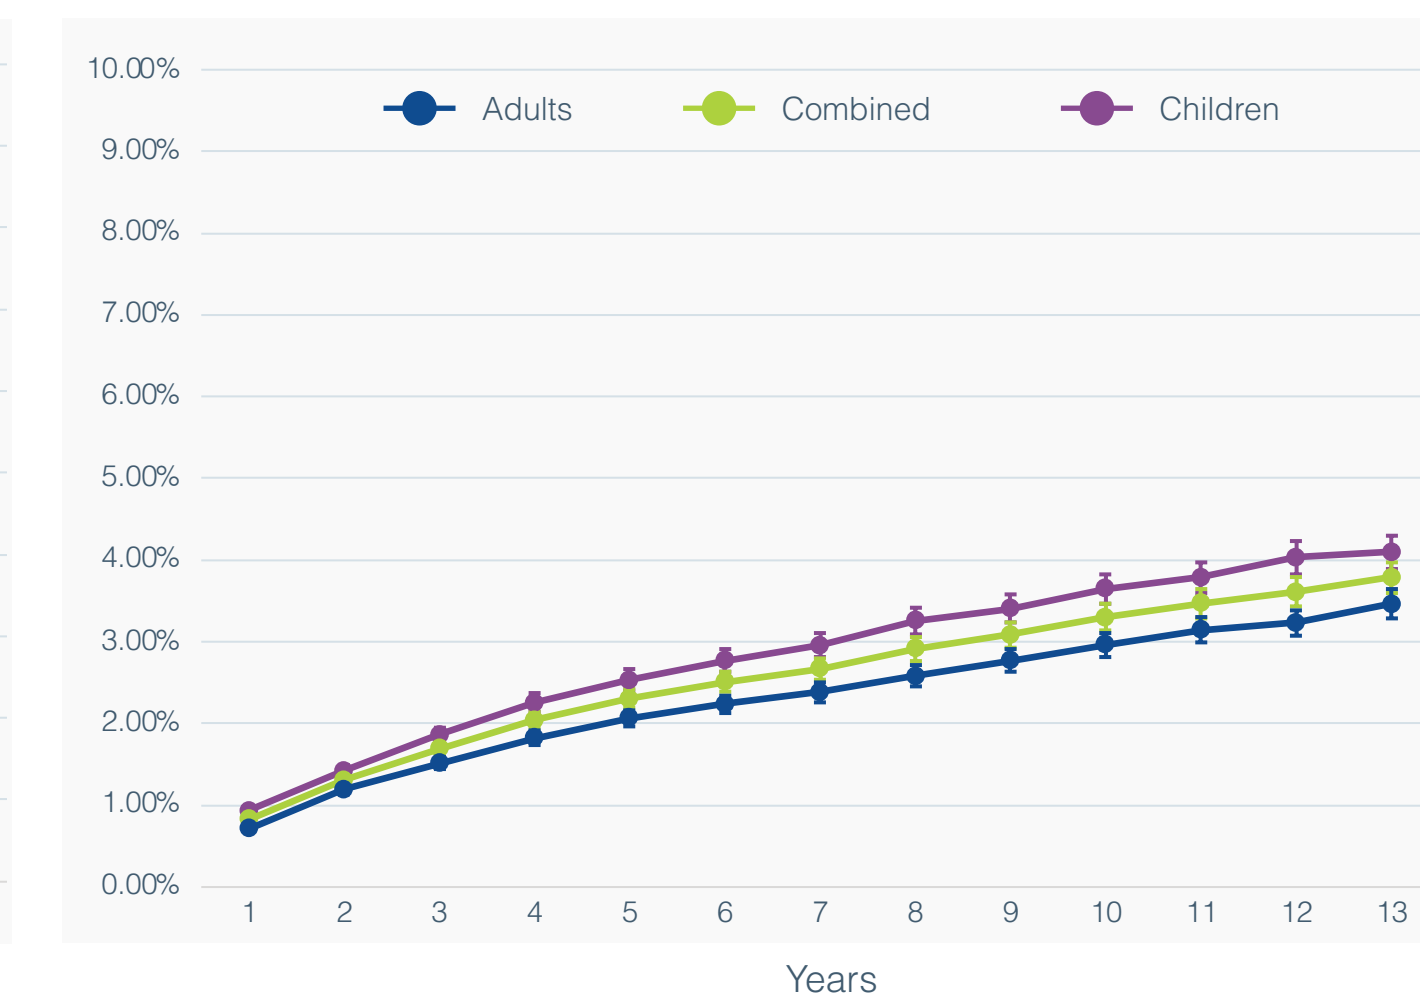

REMOVAL RATES ANALYSIS CATEGORIES
FOR CHILDREN

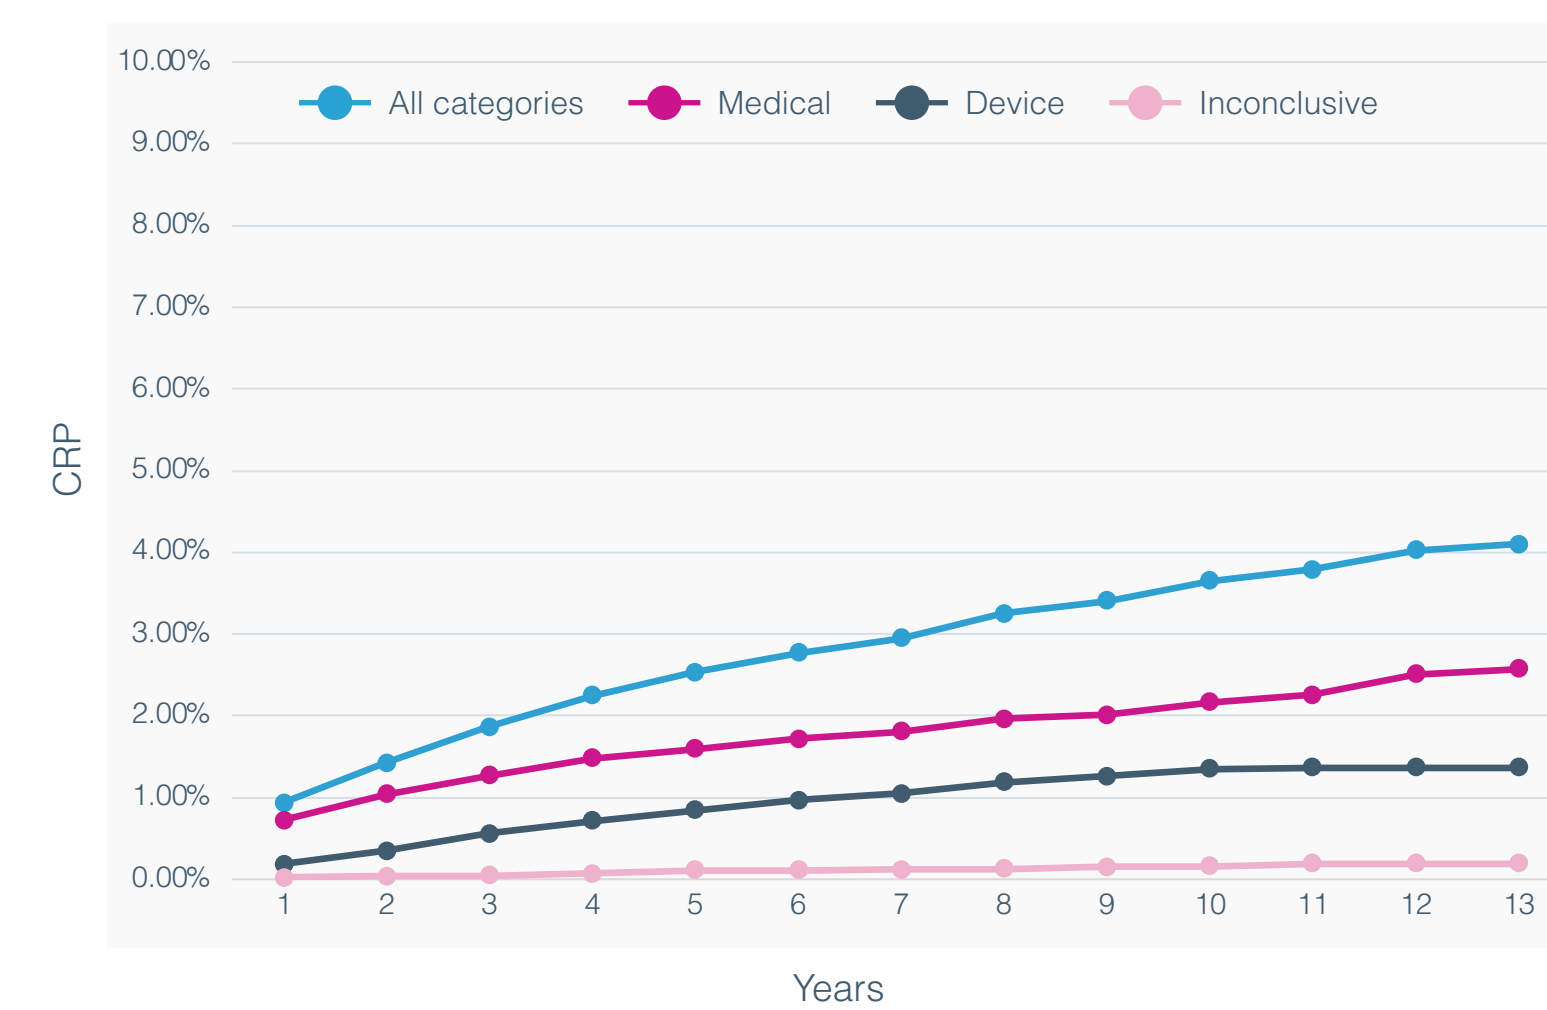

REMOVAL RATES ANALYSIS CATEGORIES
FOR ADULTS AND CHILDREN

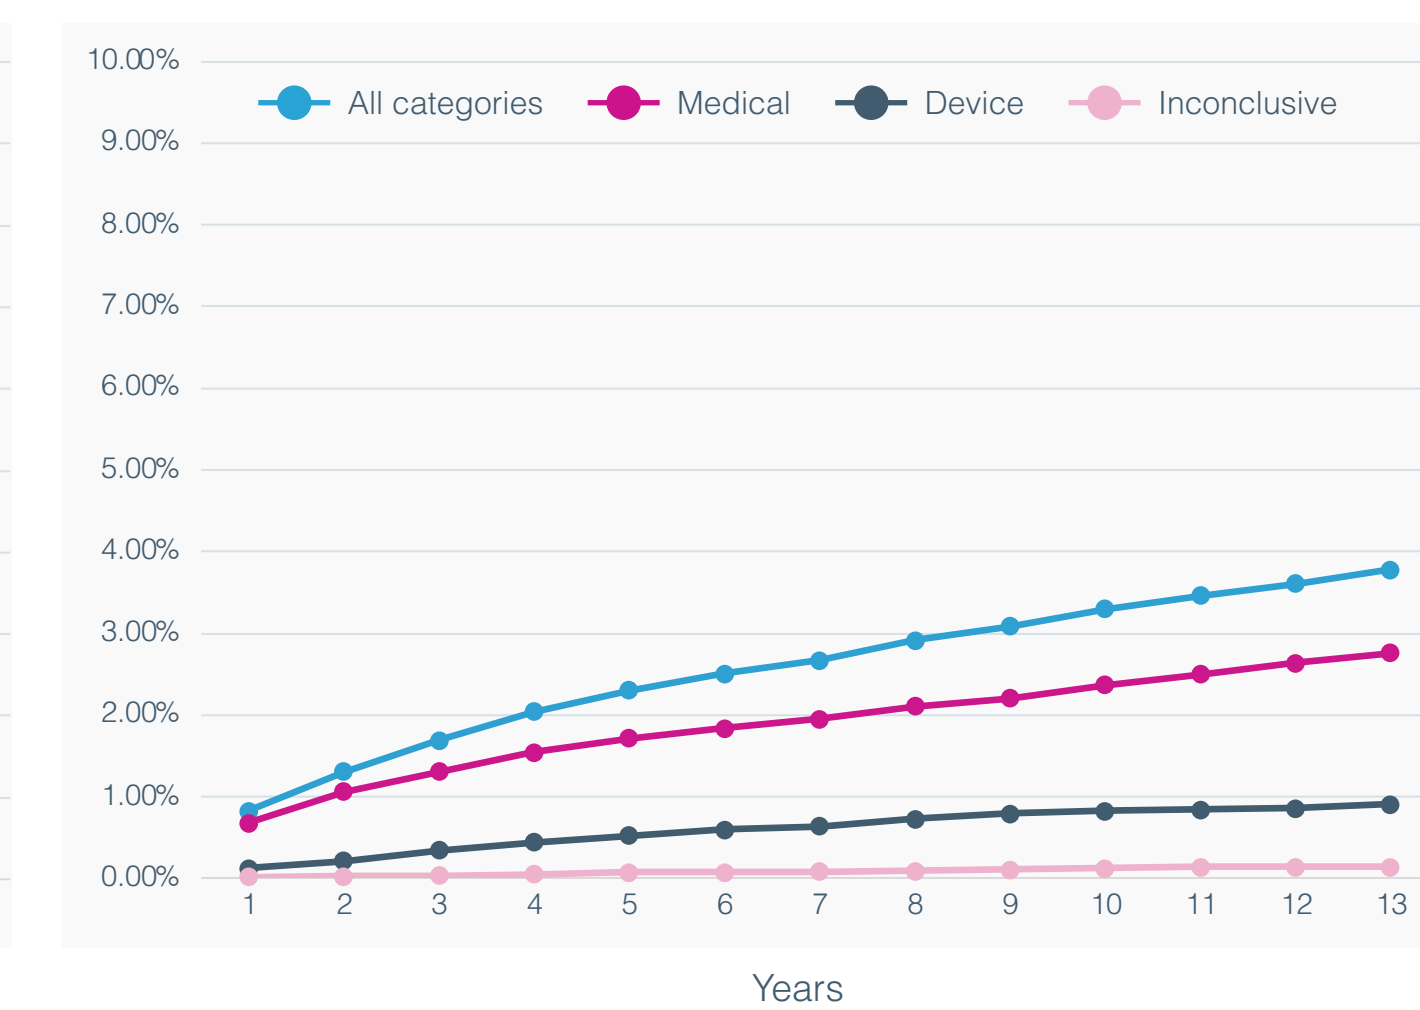

COMBINED ADULT AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	Total CI Lower
1	0.68%	0.13%	0.02%	0.83%	0.91%	0.74%
2	1.06%	0.22%	0.03%	1.31%	1.42%	1.20%
3	1.31%	0.35%	0.04%	1.69%	1.81%	1.57%
4	1.55%	0.45%	0.05%	2.04%	2.18%	1.91%
5	1.72%	0.52%	0.07%	2.30%	2.45%	2.16%
6	1.84%	0.60%	0.08%	2.51%	2.66%	2.36%
7	1.96%	0.64%	0.09%	2.67%	2.83%	2.52%
8	2.11%	0.73%	0.09%	2.92%	3.08%	2.75%
9	2.21%	0.79%	0.11%	3.09%	3.26%	2.92%
10	2.37%	0.83%	0.13%	3.30%	3.48%	3.12%
11	2.50%	0.85%	0.15%	3.47%	3.66%	3.28%
12	2.64%	0.86%	0.15%	3.61%	3.82%	3.41%
13	2.76%	0.91%	0.15%	3.78%	4.03%	3.54%

Please see the **Appendix** for a complete data set.

HIRES 90K vendor A post-mod

The HiRes 90K™ cochlear implant offers access to advanced sound coding technologies. It has undergone manufacturing modifications, with the version currently available being designated as the HiRes 90K (vendor A post-mod) implant.

NUMBER OF REGISTERED HIRES 90K IMPLANTS (VENDOR A POST-MOD)

As of April 1, 2026.
Last year of distribution: 2018.[a]

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	34662	47454	82116[b]
ANSI/AAMI CI86	40638[c]	41478	82116

a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

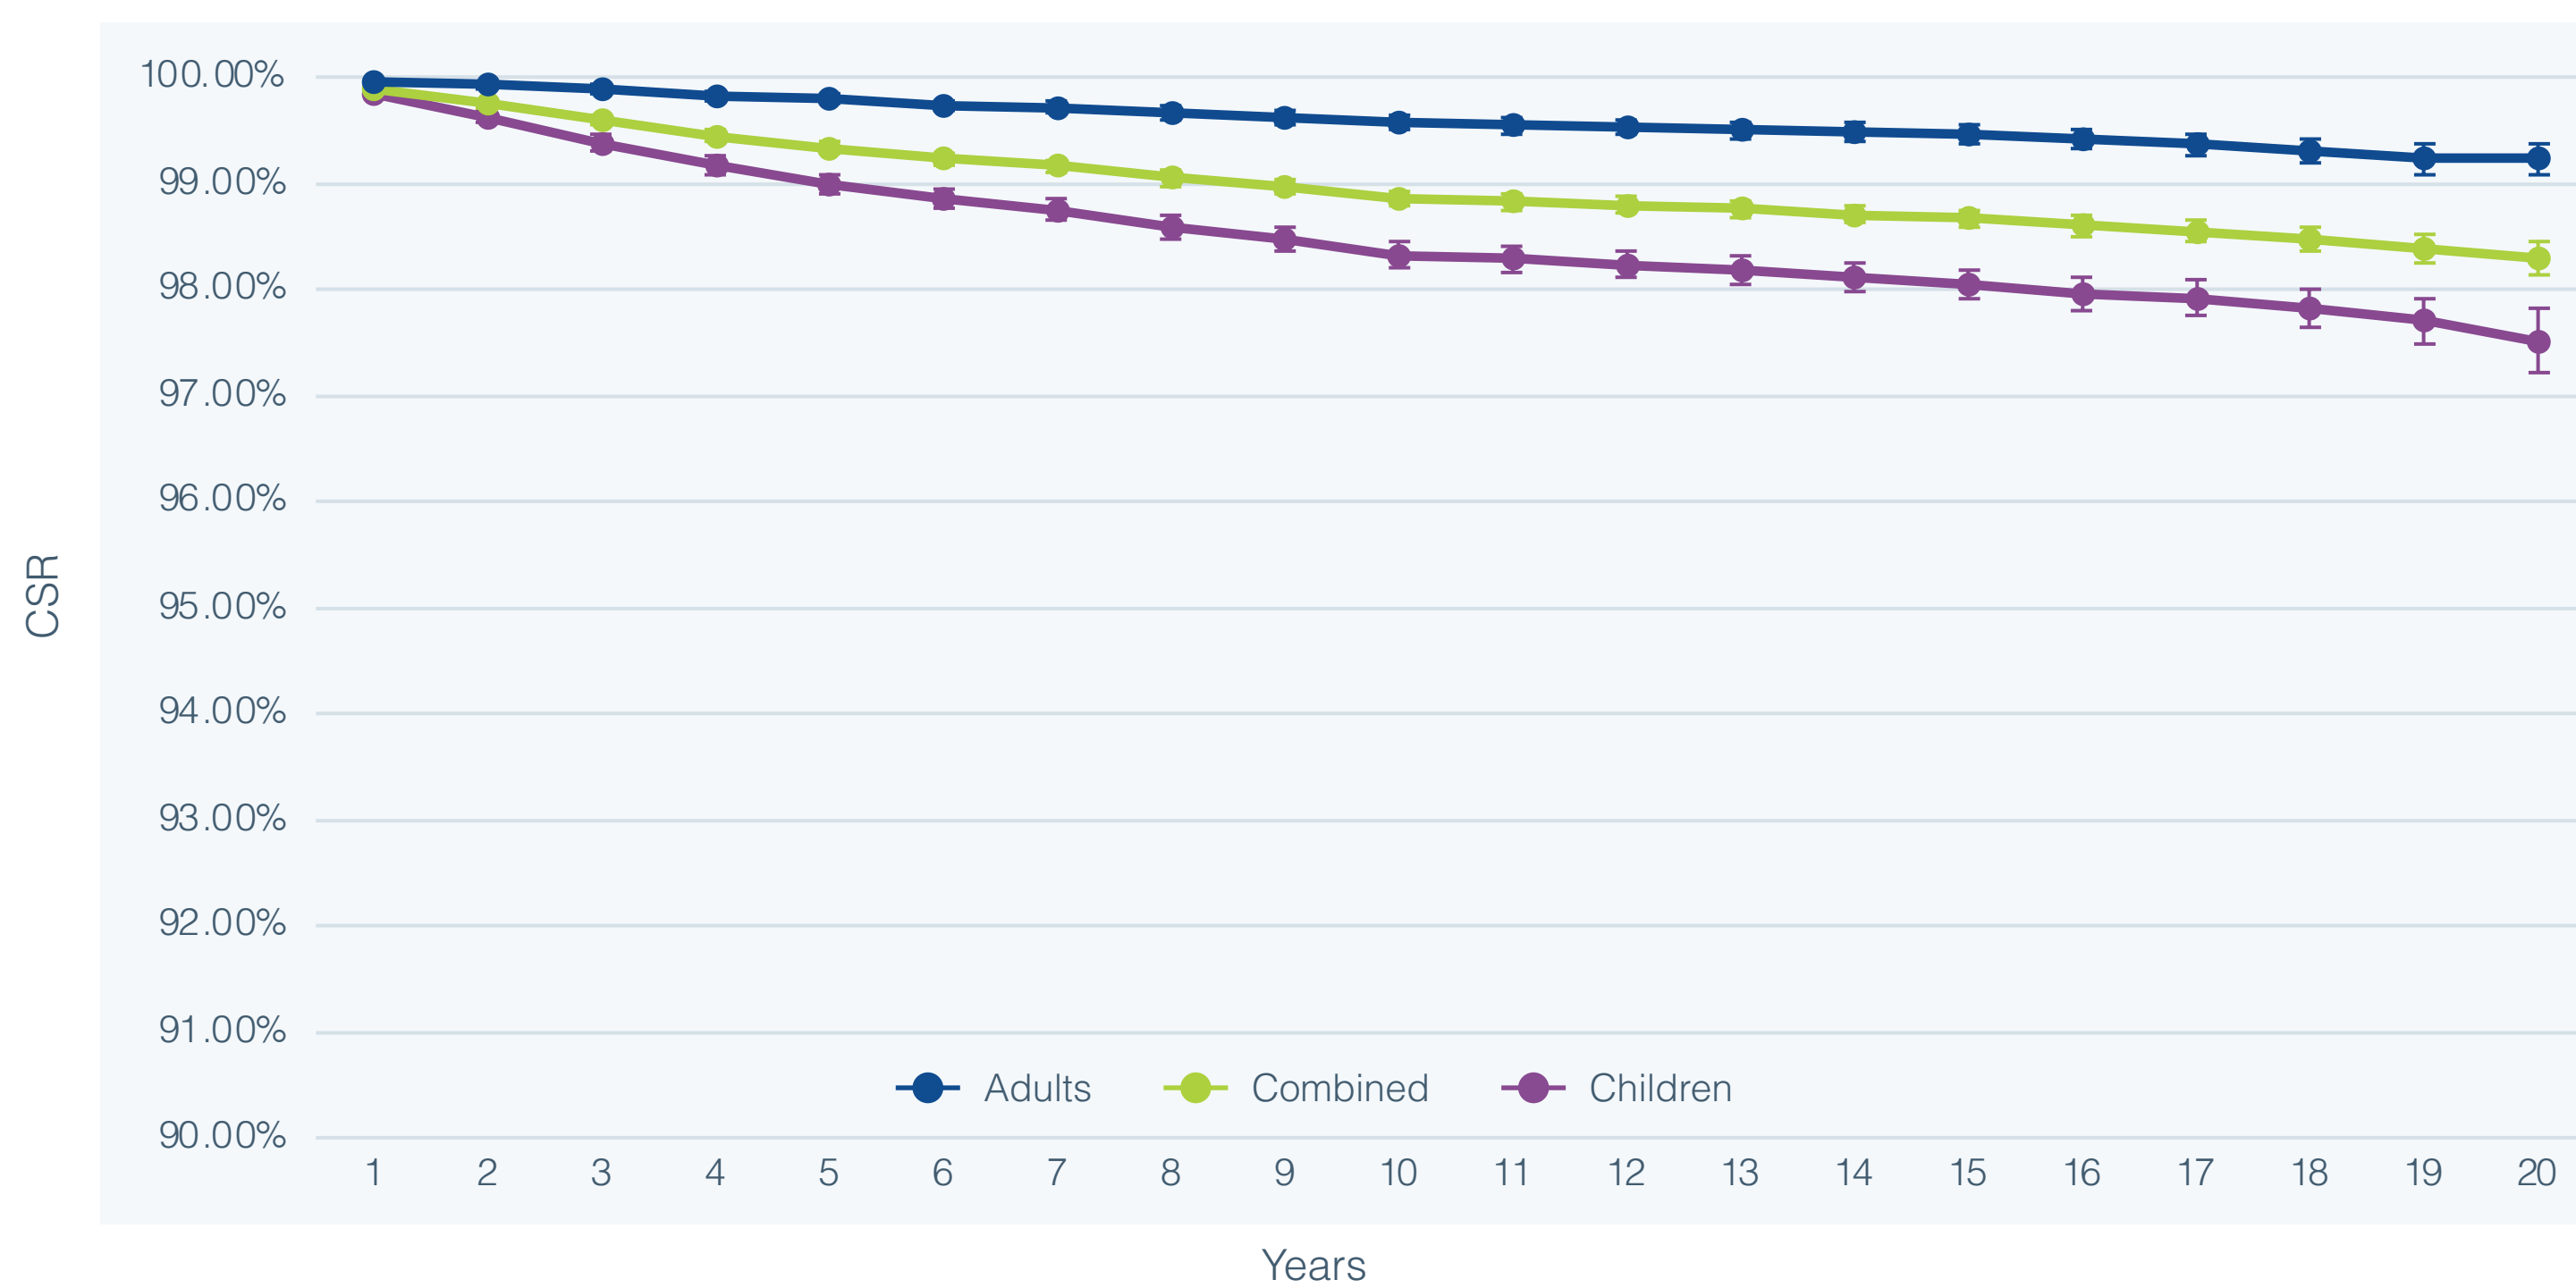

CUMULATIVE SURVIVAL RATE

Years in use	1	2	3	4	5	6	7	8	9	10
ADULTS	99.95%	99.93%	99.89%	99.83%	99.79%	99.73%	99.72%	99.67%	99.61%	99.57%
COMBINED	99.88%	99.75%	99.60%	99.45%	99.33%	99.23%	99.16%	99.05%	98.96%	98.86%
CHILDREN	99.83%	99.62%	99.38%	99.17%	98.99%	98.86%	98.76%	98.59%	98.48%	98.32%

Years in use	11	12	13	14	15	16	17	18	19	20
ADULTS	99.55%	99.53%	99.51%	99.49%	99.47%	99.42%	99.37%	99.31%	99.23%	99.23%
COMBINED	98.83%	98.79%	98.76%	98.71%	98.67%	98.60%	98.55%	98.47%	98.38%	98.30%
CHILDREN	98.29%	98.24%	98.19%	98.12%	98.05%	97.96%	97.92%	97.82%	97.71%	97.51%

ANSI/AAMI CI86

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

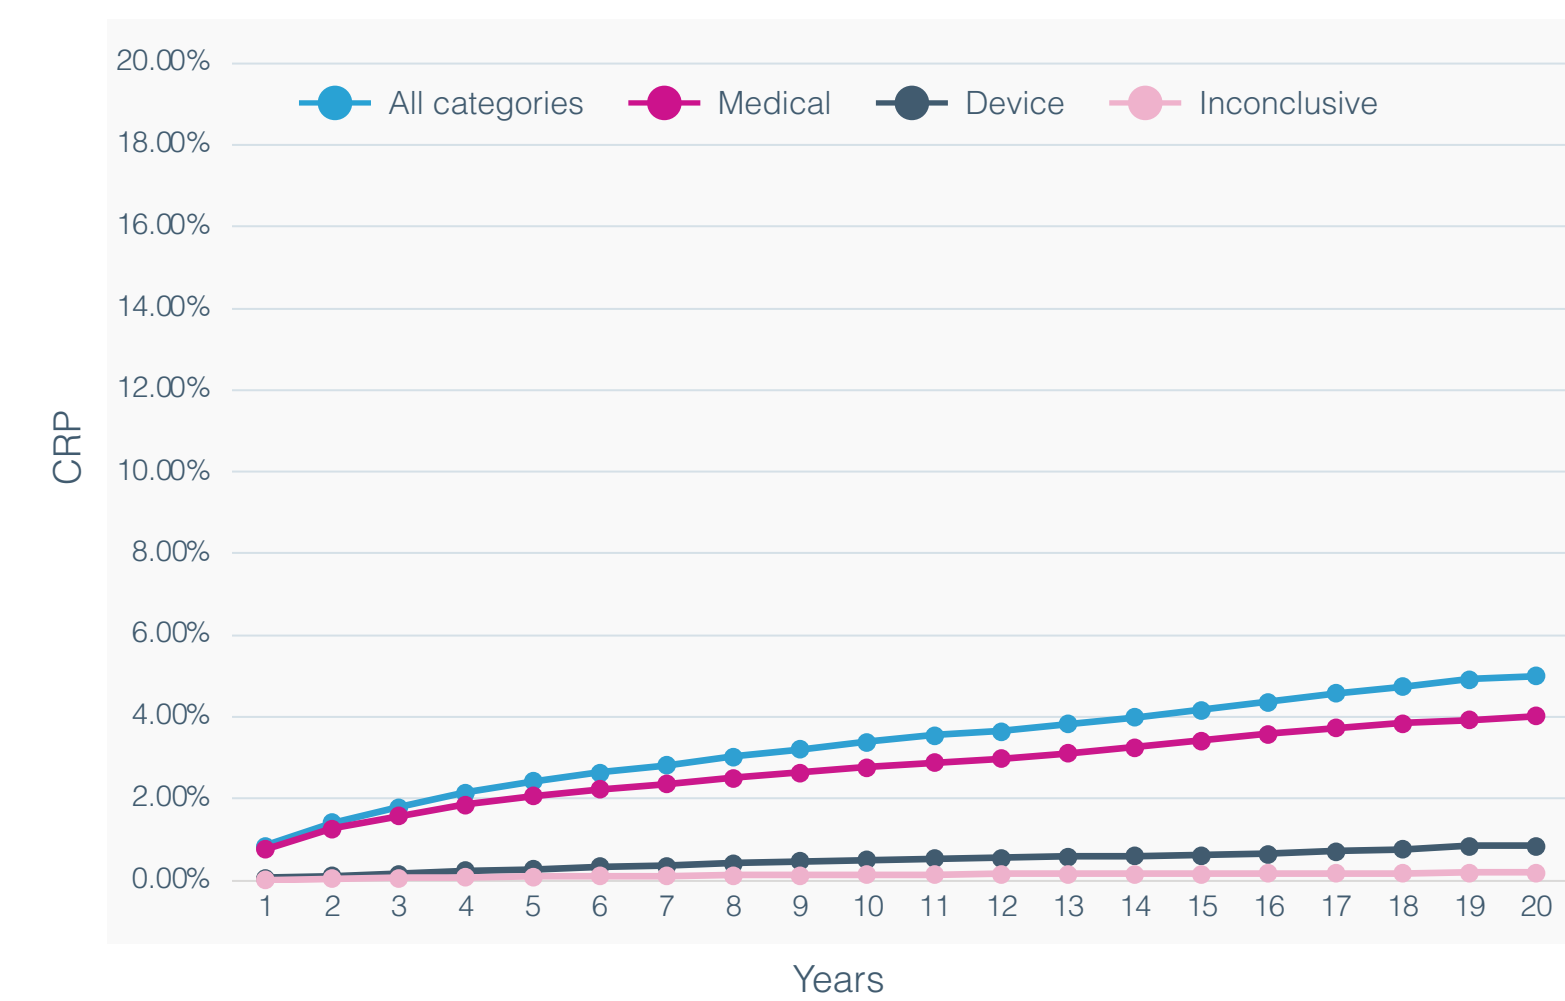

REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

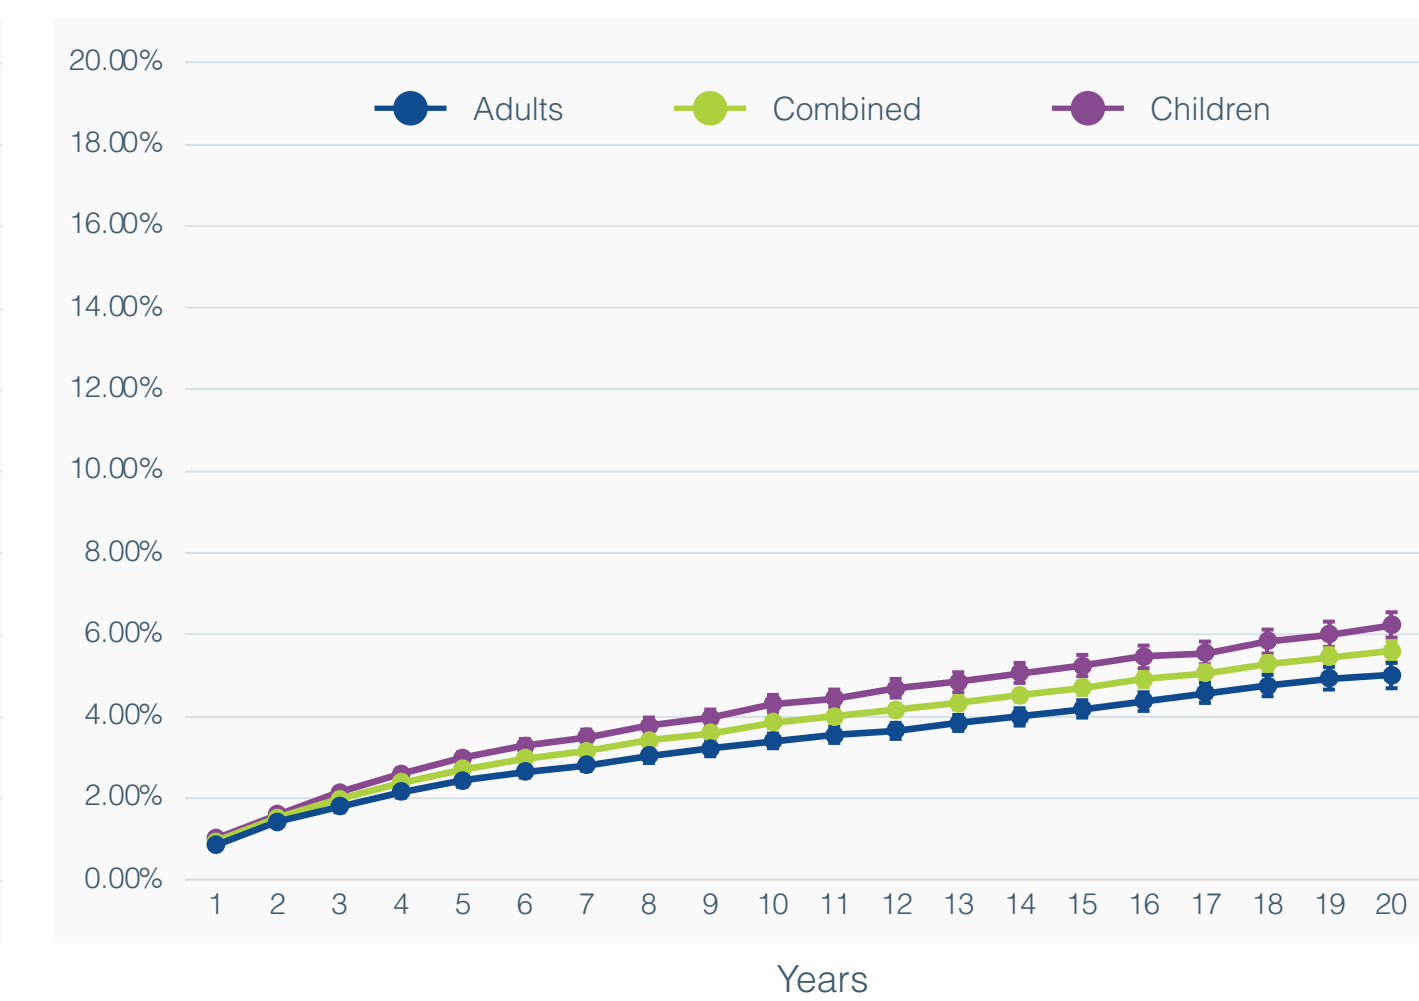

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

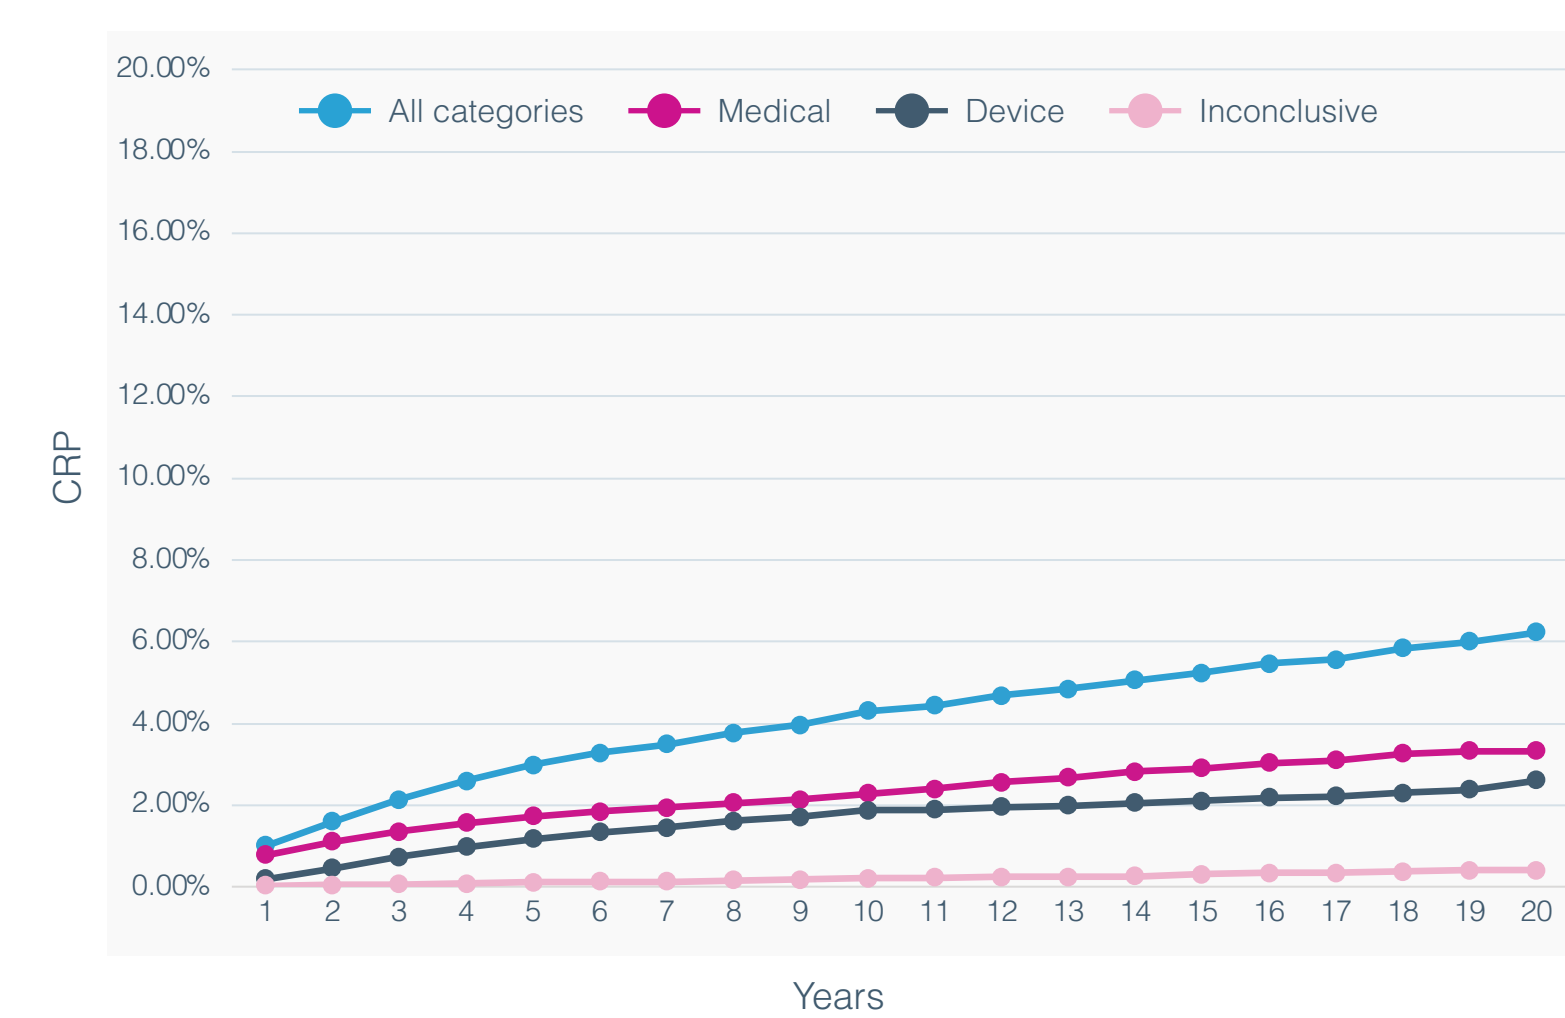

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

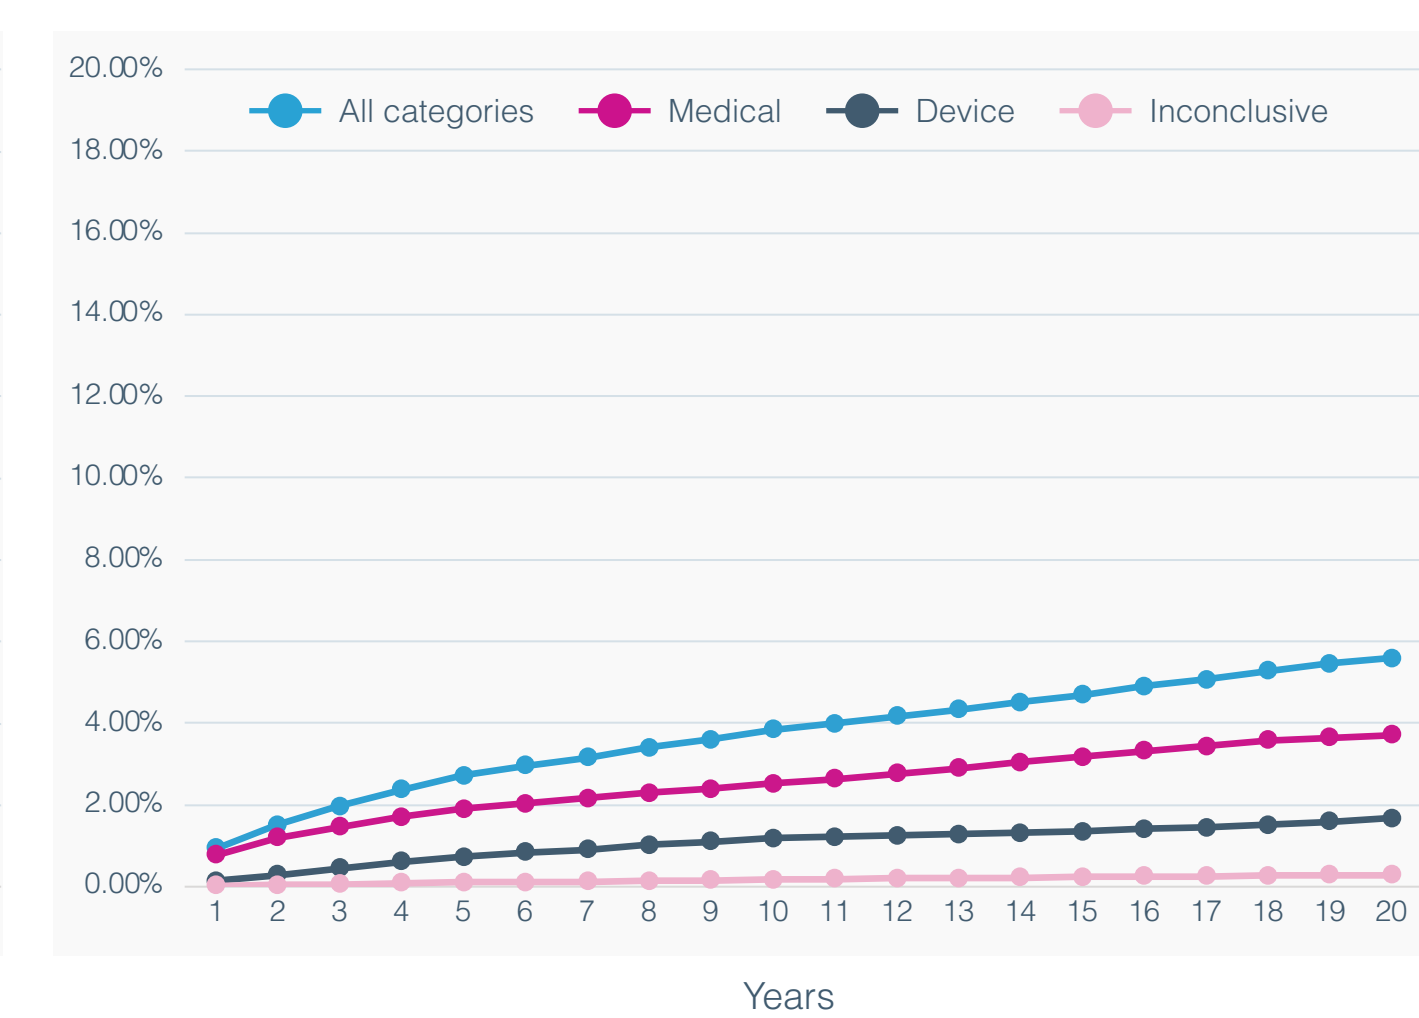

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	Total CI Lower
1	0.78%	0.13%	0.02%	0.93%	0.99%	0.86%
2	1.19%	0.28%	0.04%	1.51%	1.59%	1.42%
3	1.46%	0.45%	0.06%	1.96%	2.06%	1.87%
4	1.70%	0.61%	0.08%	2.37%	2.48%	2.27%
5	1.90%	0.73%	0.10%	2.71%	2.82%	2.60%
6	2.03%	0.84%	0.11%	2.96%	3.08%	2.84%
7	2.15%	0.91%	0.12%	3.15%	3.27%	3.03%
8	2.28%	1.02%	0.13%	3.40%	3.53%	3.28%
9	2.38%	1.09%	0.15%	3.59%	3.72%	3.46%
10	2.52%	1.18%	0.17%	3.84%	3.98%	3.71%
11	2.64%	1.21%	0.18%	3.99%	4.13%	3.85%
12	2.76%	1.24%	0.20%	4.16%	4.30%	4.02%
13	2.89%	1.28%	0.20%	4.33%	4.48%	4.18%
14	3.03%	1.31%	0.21%	4.51%	4.67%	4.35%
15	3.17%	1.34%	0.23%	4.69%	4.86%	4.53%
16	3.31%	1.40%	0.24%	4.90%	5.08%	4.73%
17	3.43%	1.45%	0.24%	5.06%	5.24%	4.88%
18	3.57%	1.51%	0.26%	5.28%	5.48%	5.08%
19	3.65%	1.59%	0.29%	5.45%	5.67%	5.23%
20	3.70%	1.68%	0.29%	5.59%	5.84%	5.34%

Please see the **Appendix** for a complete data set.

HIRES 90K vendor A all

NUMBER OF REGISTERED HIRES 90K IMPLANTS (VENDOR A ALL)

As of April 1, 2026.
Last year of distribution: 2018.[a]

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	36113	48554	84667[b]
ANSI/AAMI CI86	42299[c]	42368	84667

a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

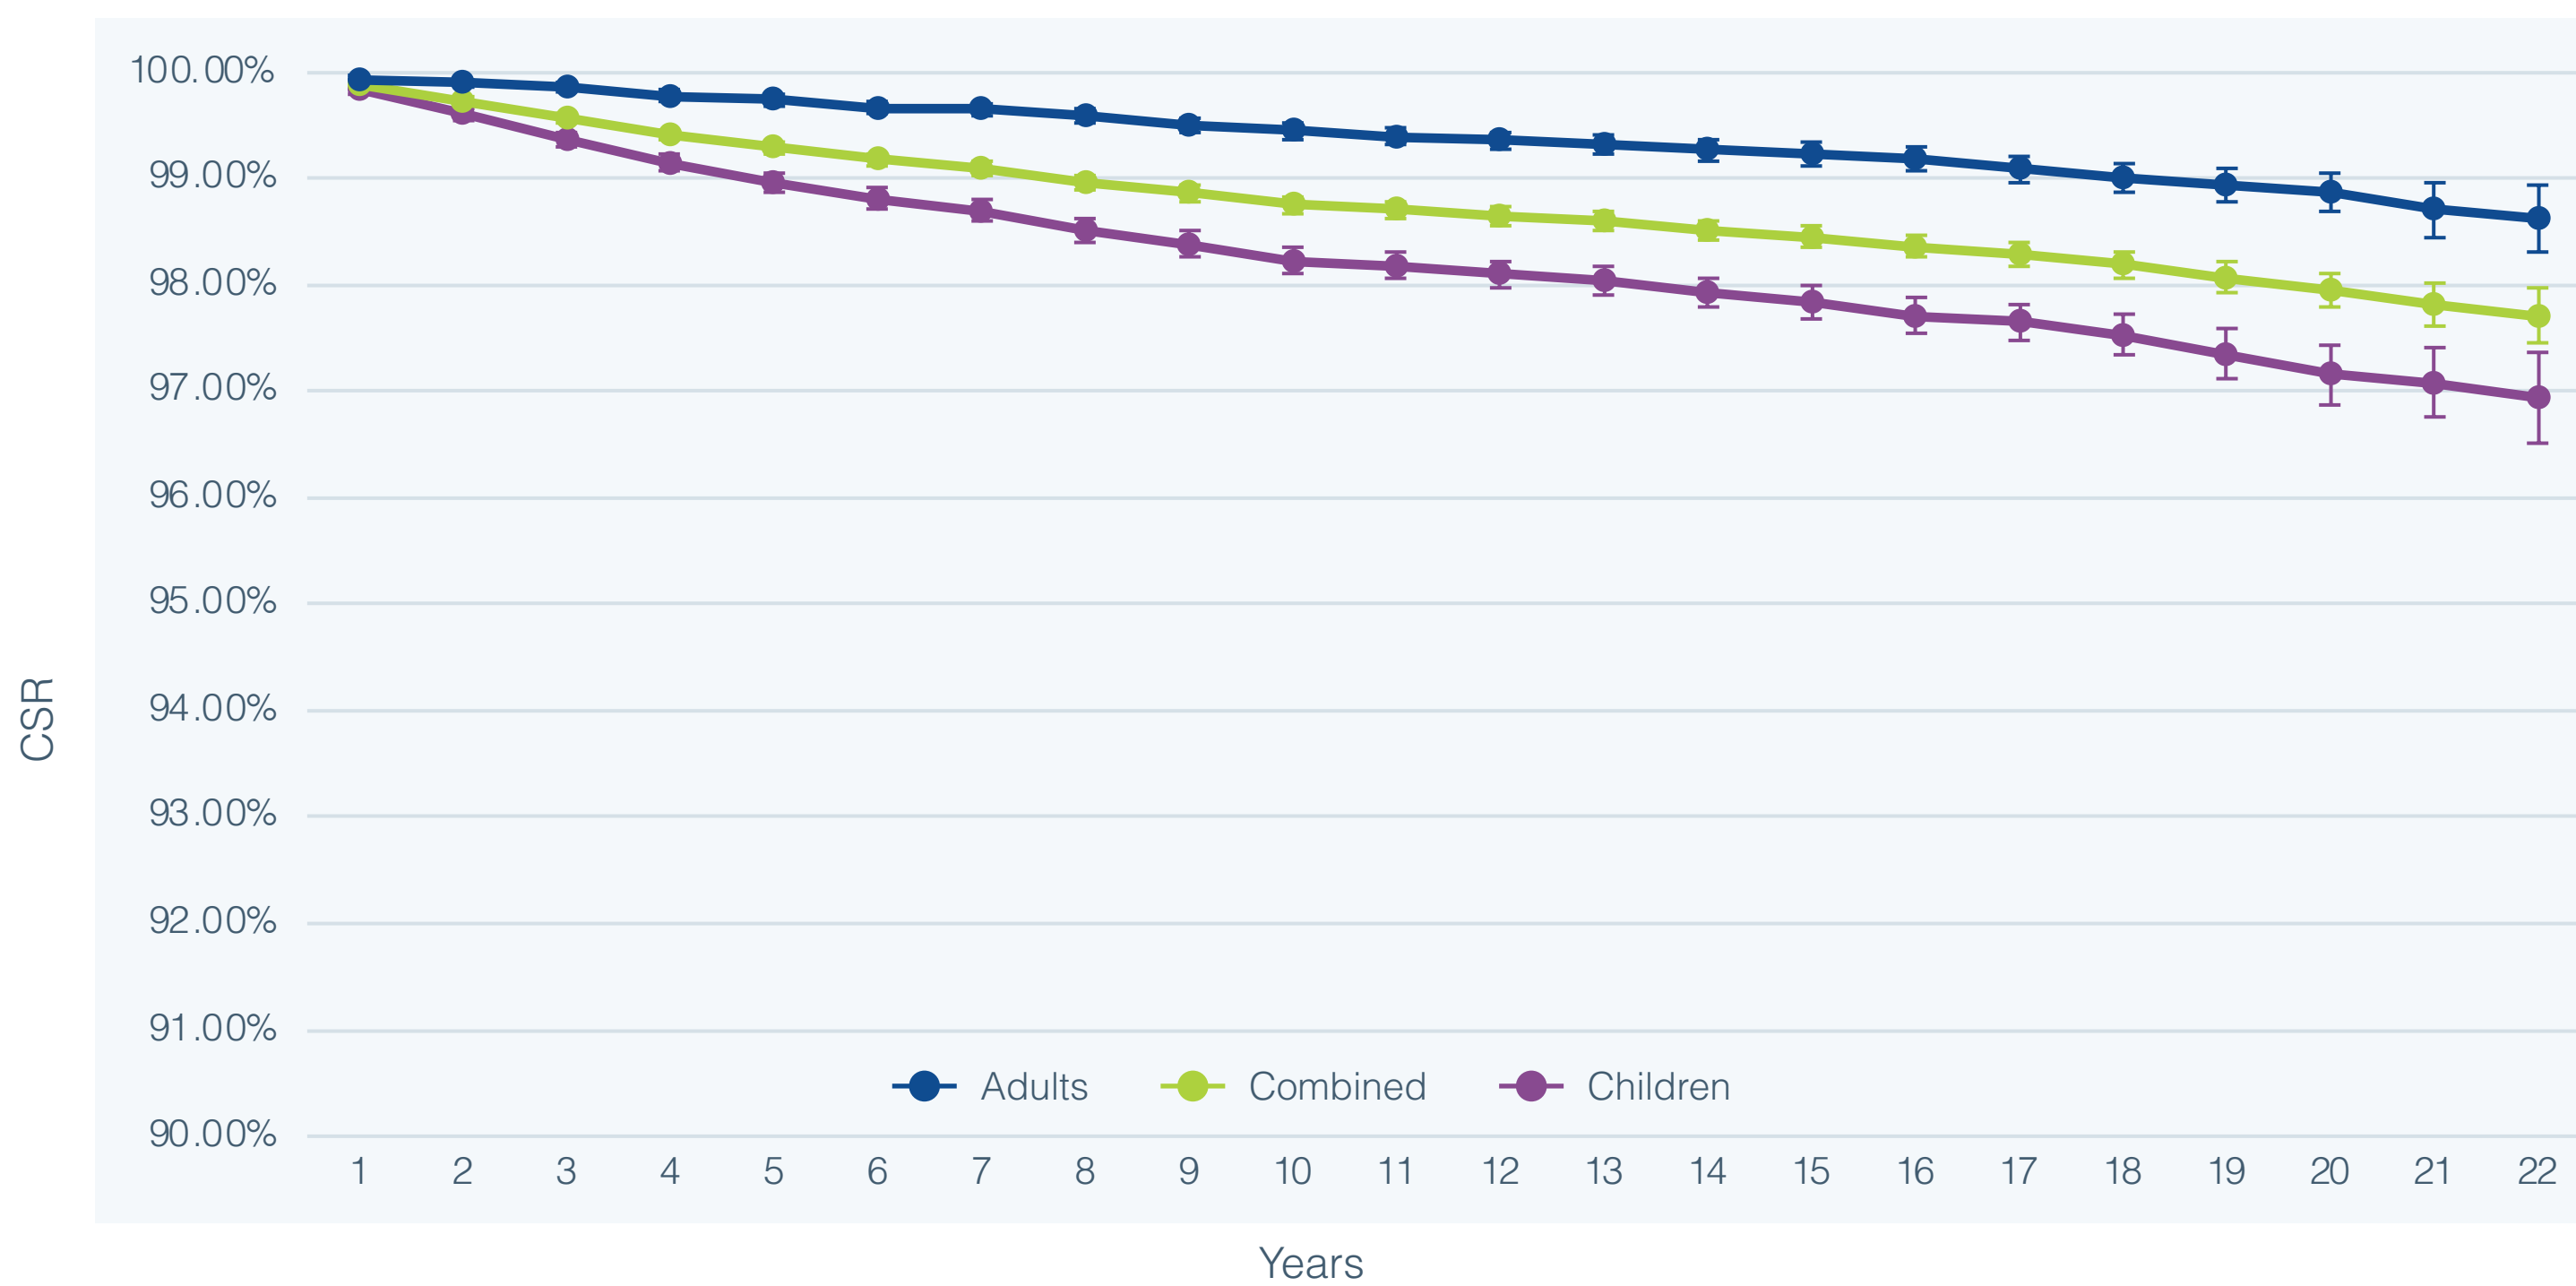

CUMULATIVE SURVIVAL RATE

Years in use	1	2	3	4	5	6	7	8	9	10	11
ADULTS	99.94%	99.90%	99.86%	99.78%	99.74%	99.67%	99.65%	99.58%	99.50%	99.45%	99.40%
COMBINED	99.87%	99.73%	99.57%	99.41%	99.29%	99.18%	99.10%	98.97%	98.87%	98.76%	98.71%
CHILDREN	99.83%	99.61%	99.36%	99.15%	98.95%	98.81%	98.70%	98.51%	98.39%	98.23%	98.18%

Years in use	12	13	14	15	16	17	18	19	20	21	22
ADULTS	99.36%	99.32%	99.27%	99.23%	99.18%	99.09%	99.01%	98.94%	98.88%	98.71%	98.62%
COMBINED	98.64%	98.60%	98.52%	98.45%	98.36%	98.29%	98.19%	98.07%	97.95%	97.82%	97.71%
CHILDREN	98.10%	98.04%	97.93%	97.84%	97.71%	97.65%	97.53%	97.35%	97.15%	97.08%	96.94%

ANSI/AAMI CI86

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

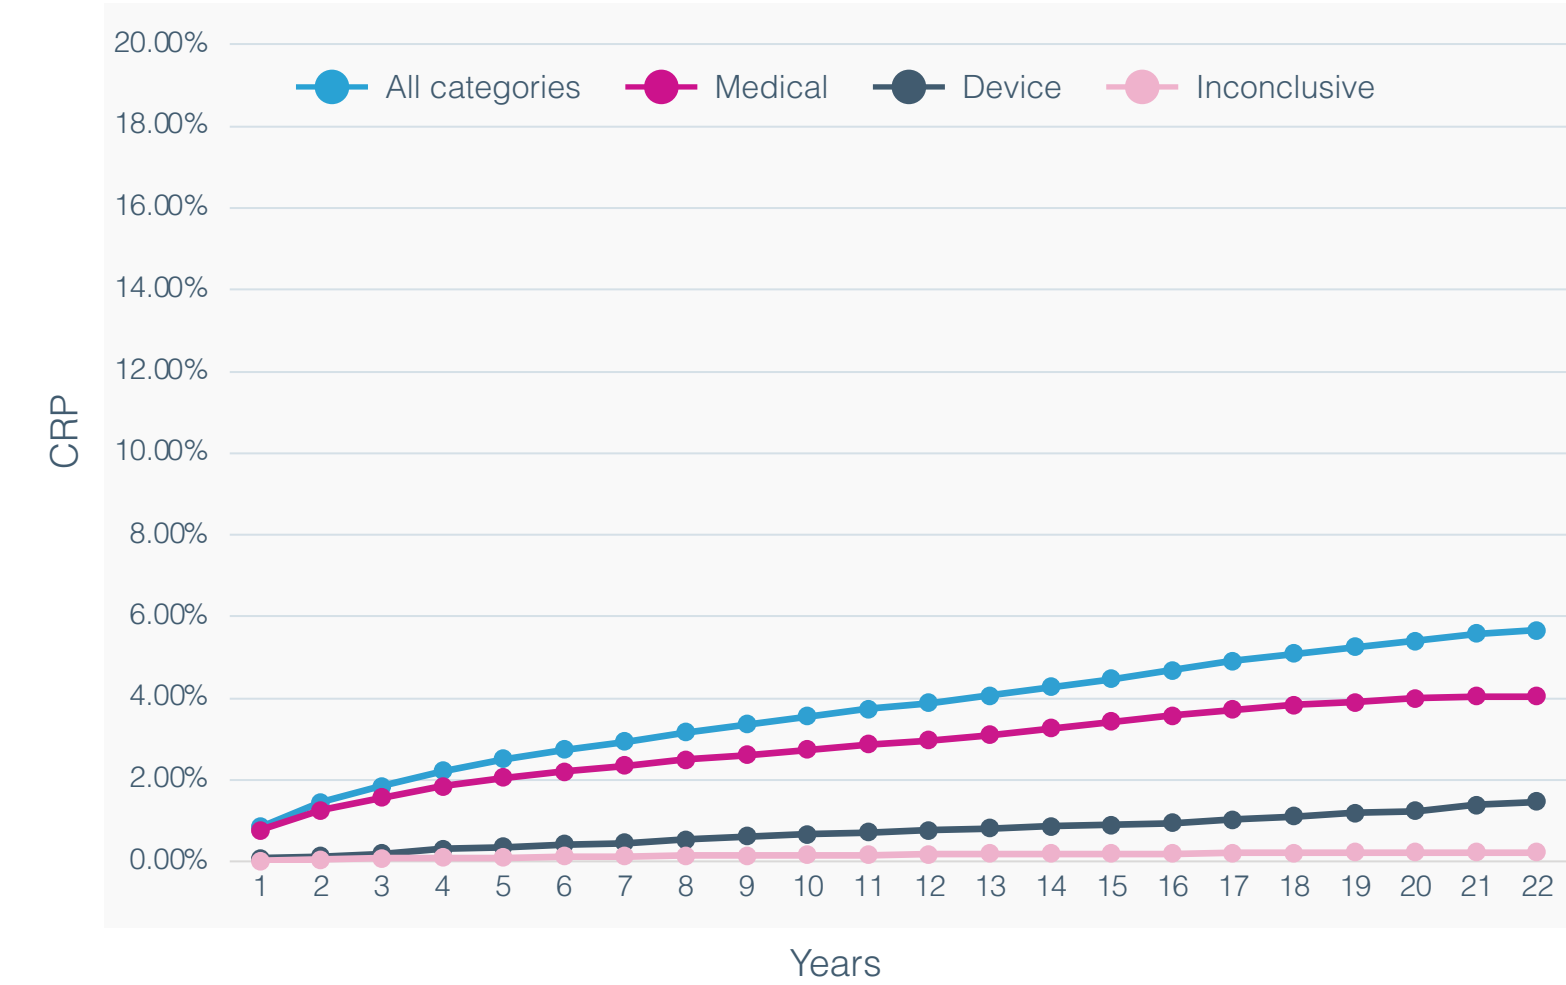

REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

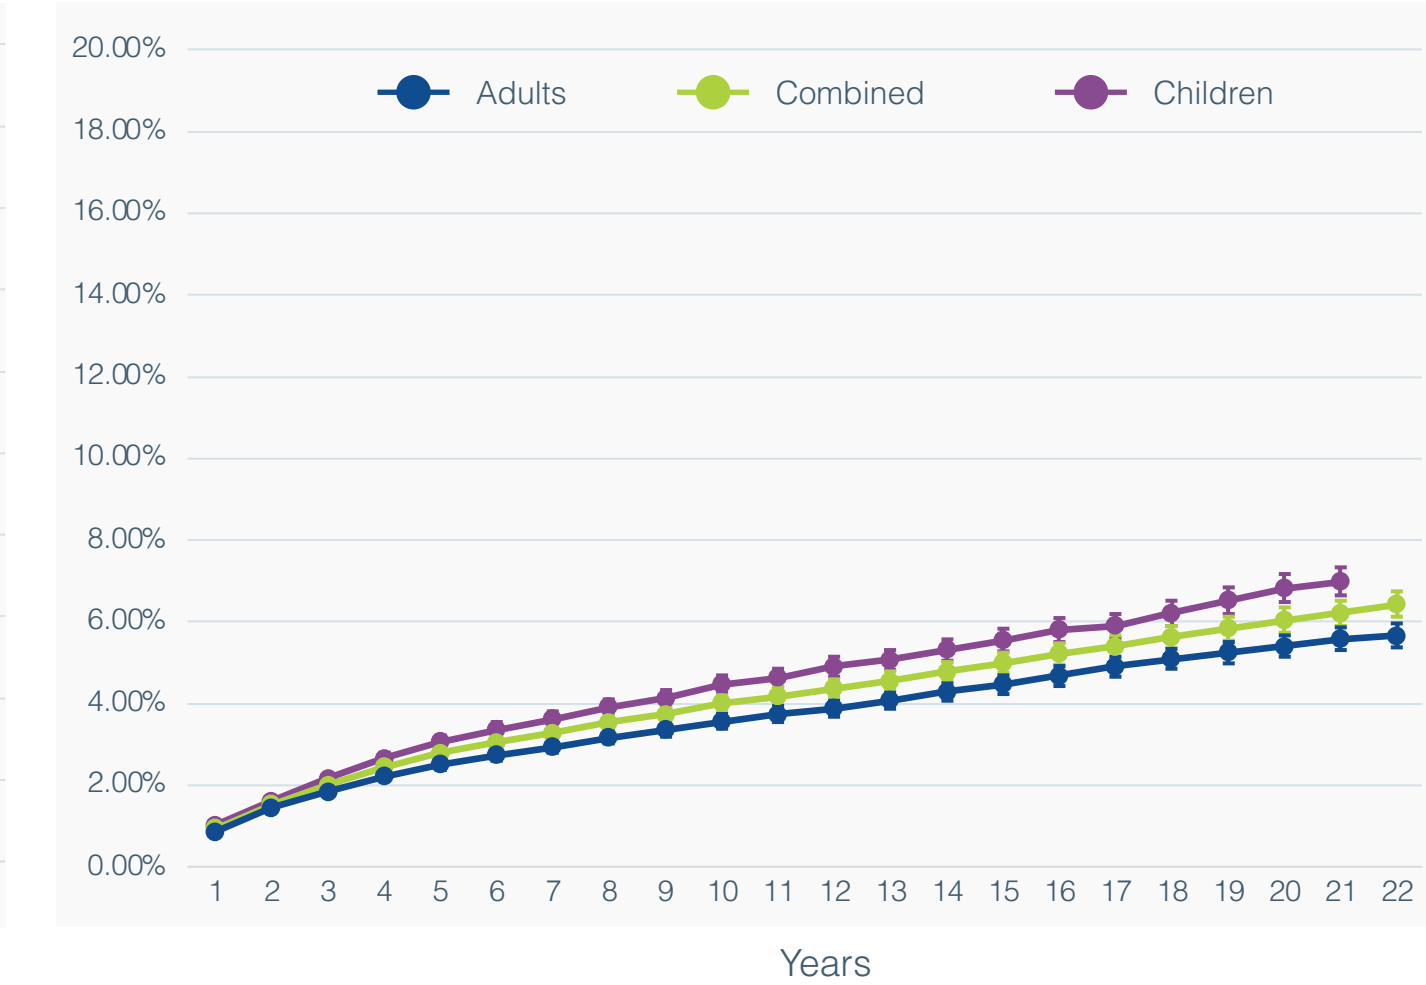

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

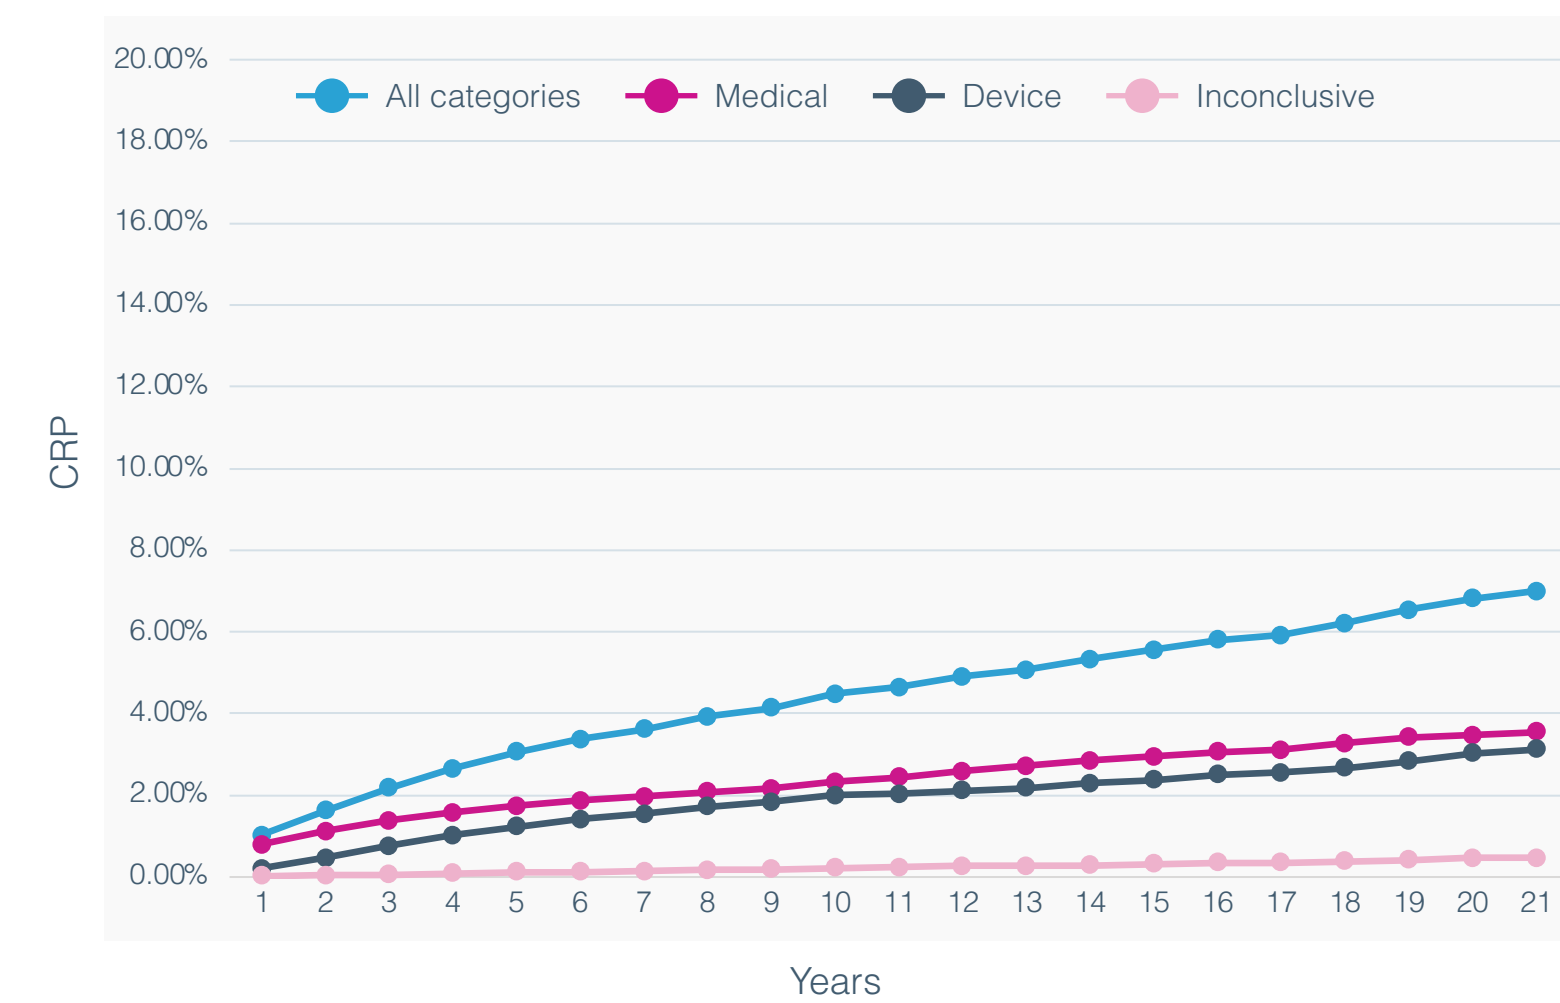

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

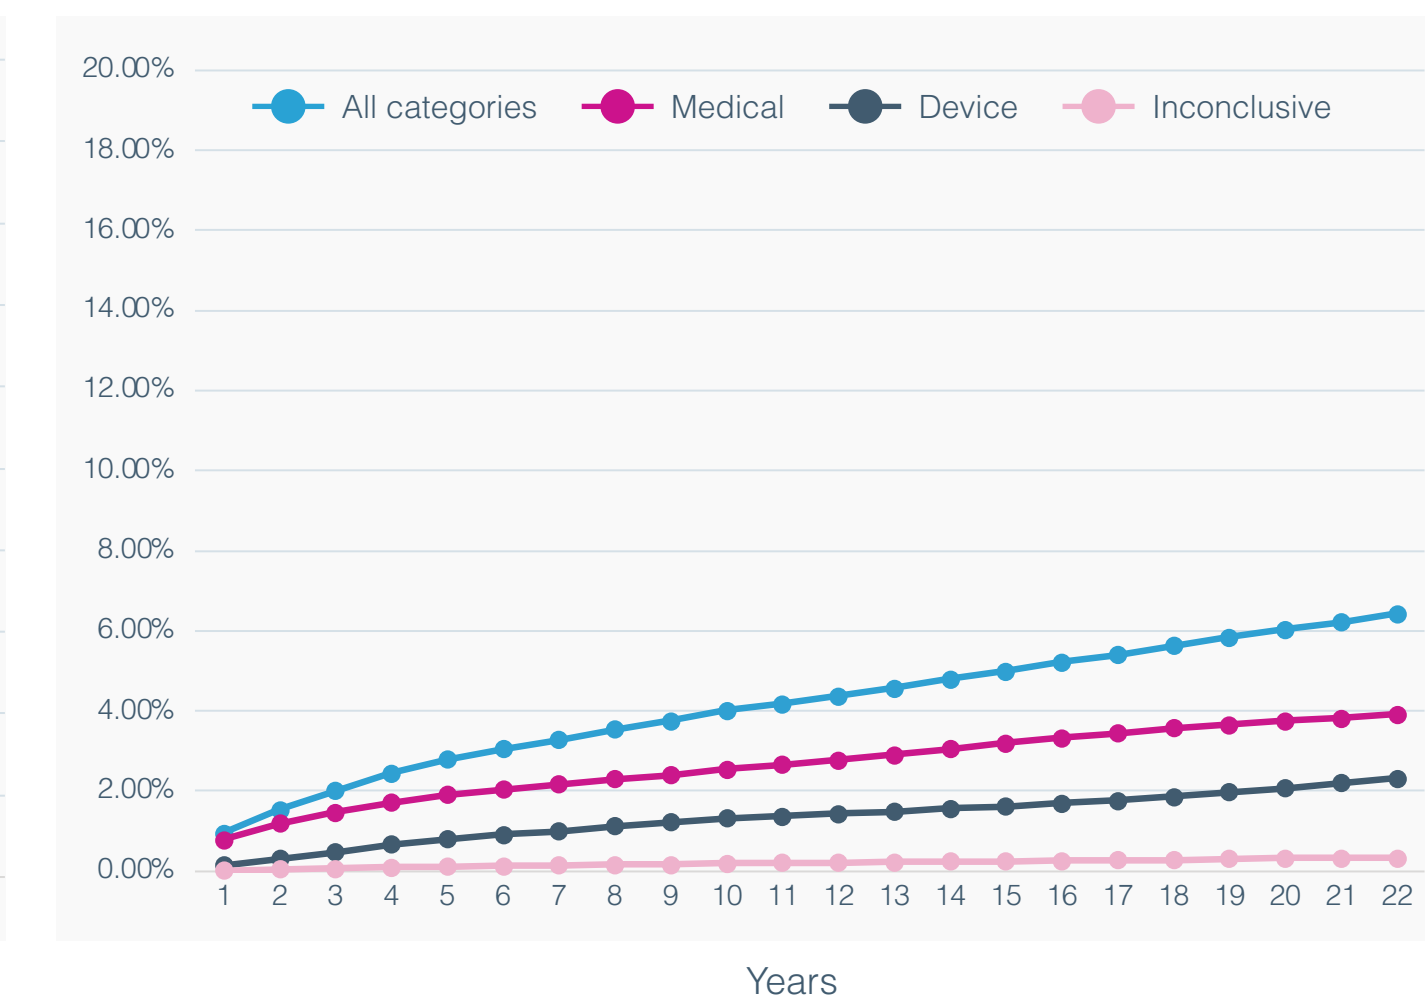

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	Total CI Lower
1	0.78%	0.14%	0.02%	0.94%	1.01%	0.88%
2	1.19%	0.30%	0.04%	1.53%	1.62%	1.45%
3	1.47%	0.48%	0.07%	2.01%	2.10%	1.91%
4	1.71%	0.66%	0.09%	2.44%	2.54%	2.34%
5	1.90%	0.79%	0.11%	2.79%	2.90%	2.67%
6	2.03%	0.92%	0.12%	3.05%	3.17%	2.94%
7	2.16%	1.00%	0.14%	3.27%	3.39%	3.15%
8	2.29%	1.13%	0.15%	3.54%	3.67%	3.42%
9	2.39%	1.22%	0.17%	3.74%	3.87%	3.61%
10	2.54%	1.33%	0.19%	4.01%	4.15%	3.87%
11	2.65%	1.37%	0.20%	4.18%	4.32%	4.04%
12	2.78%	1.43%	0.22%	4.38%	4.52%	4.23%
13	2.91%	1.48%	0.22%	4.56%	4.71%	4.41%
14	3.05%	1.56%	0.23%	4.79%	4.94%	4.63%
15	3.19%	1.61%	0.25%	4.99%	5.16%	4.82%
16	3.33%	1.69%	0.26%	5.21%	5.39%	5.04%
17	3.44%	1.77%	0.27%	5.40%	5.58%	5.21%
18	3.57%	1.86%	0.28%	5.63%	5.83%	5.43%
19	3.66%	1.97%	0.30%	5.84%	6.06%	5.62%
20	3.75%	2.07%	0.32%	6.04%	6.28%	5.79%
21	3.81%	2.20%	0.32%	6.22%	6.51%	5.94%
22	3.92%	2.31%	0.32%	6.43%	6.79%	6.08%

Please see the **Appendix** for a complete data set.

HIRES 90K vendor A pre-mod

NUMBER OF REGISTERED HIRES 90K IMPLANTS (VENDOR A PRE-MOD)

As of April 1, 2026.
Last year of distribution: 2005.[a]

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	1451	1100	2551[b]
ANSI/AAMI CI86	1661[c]	890	2551

a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

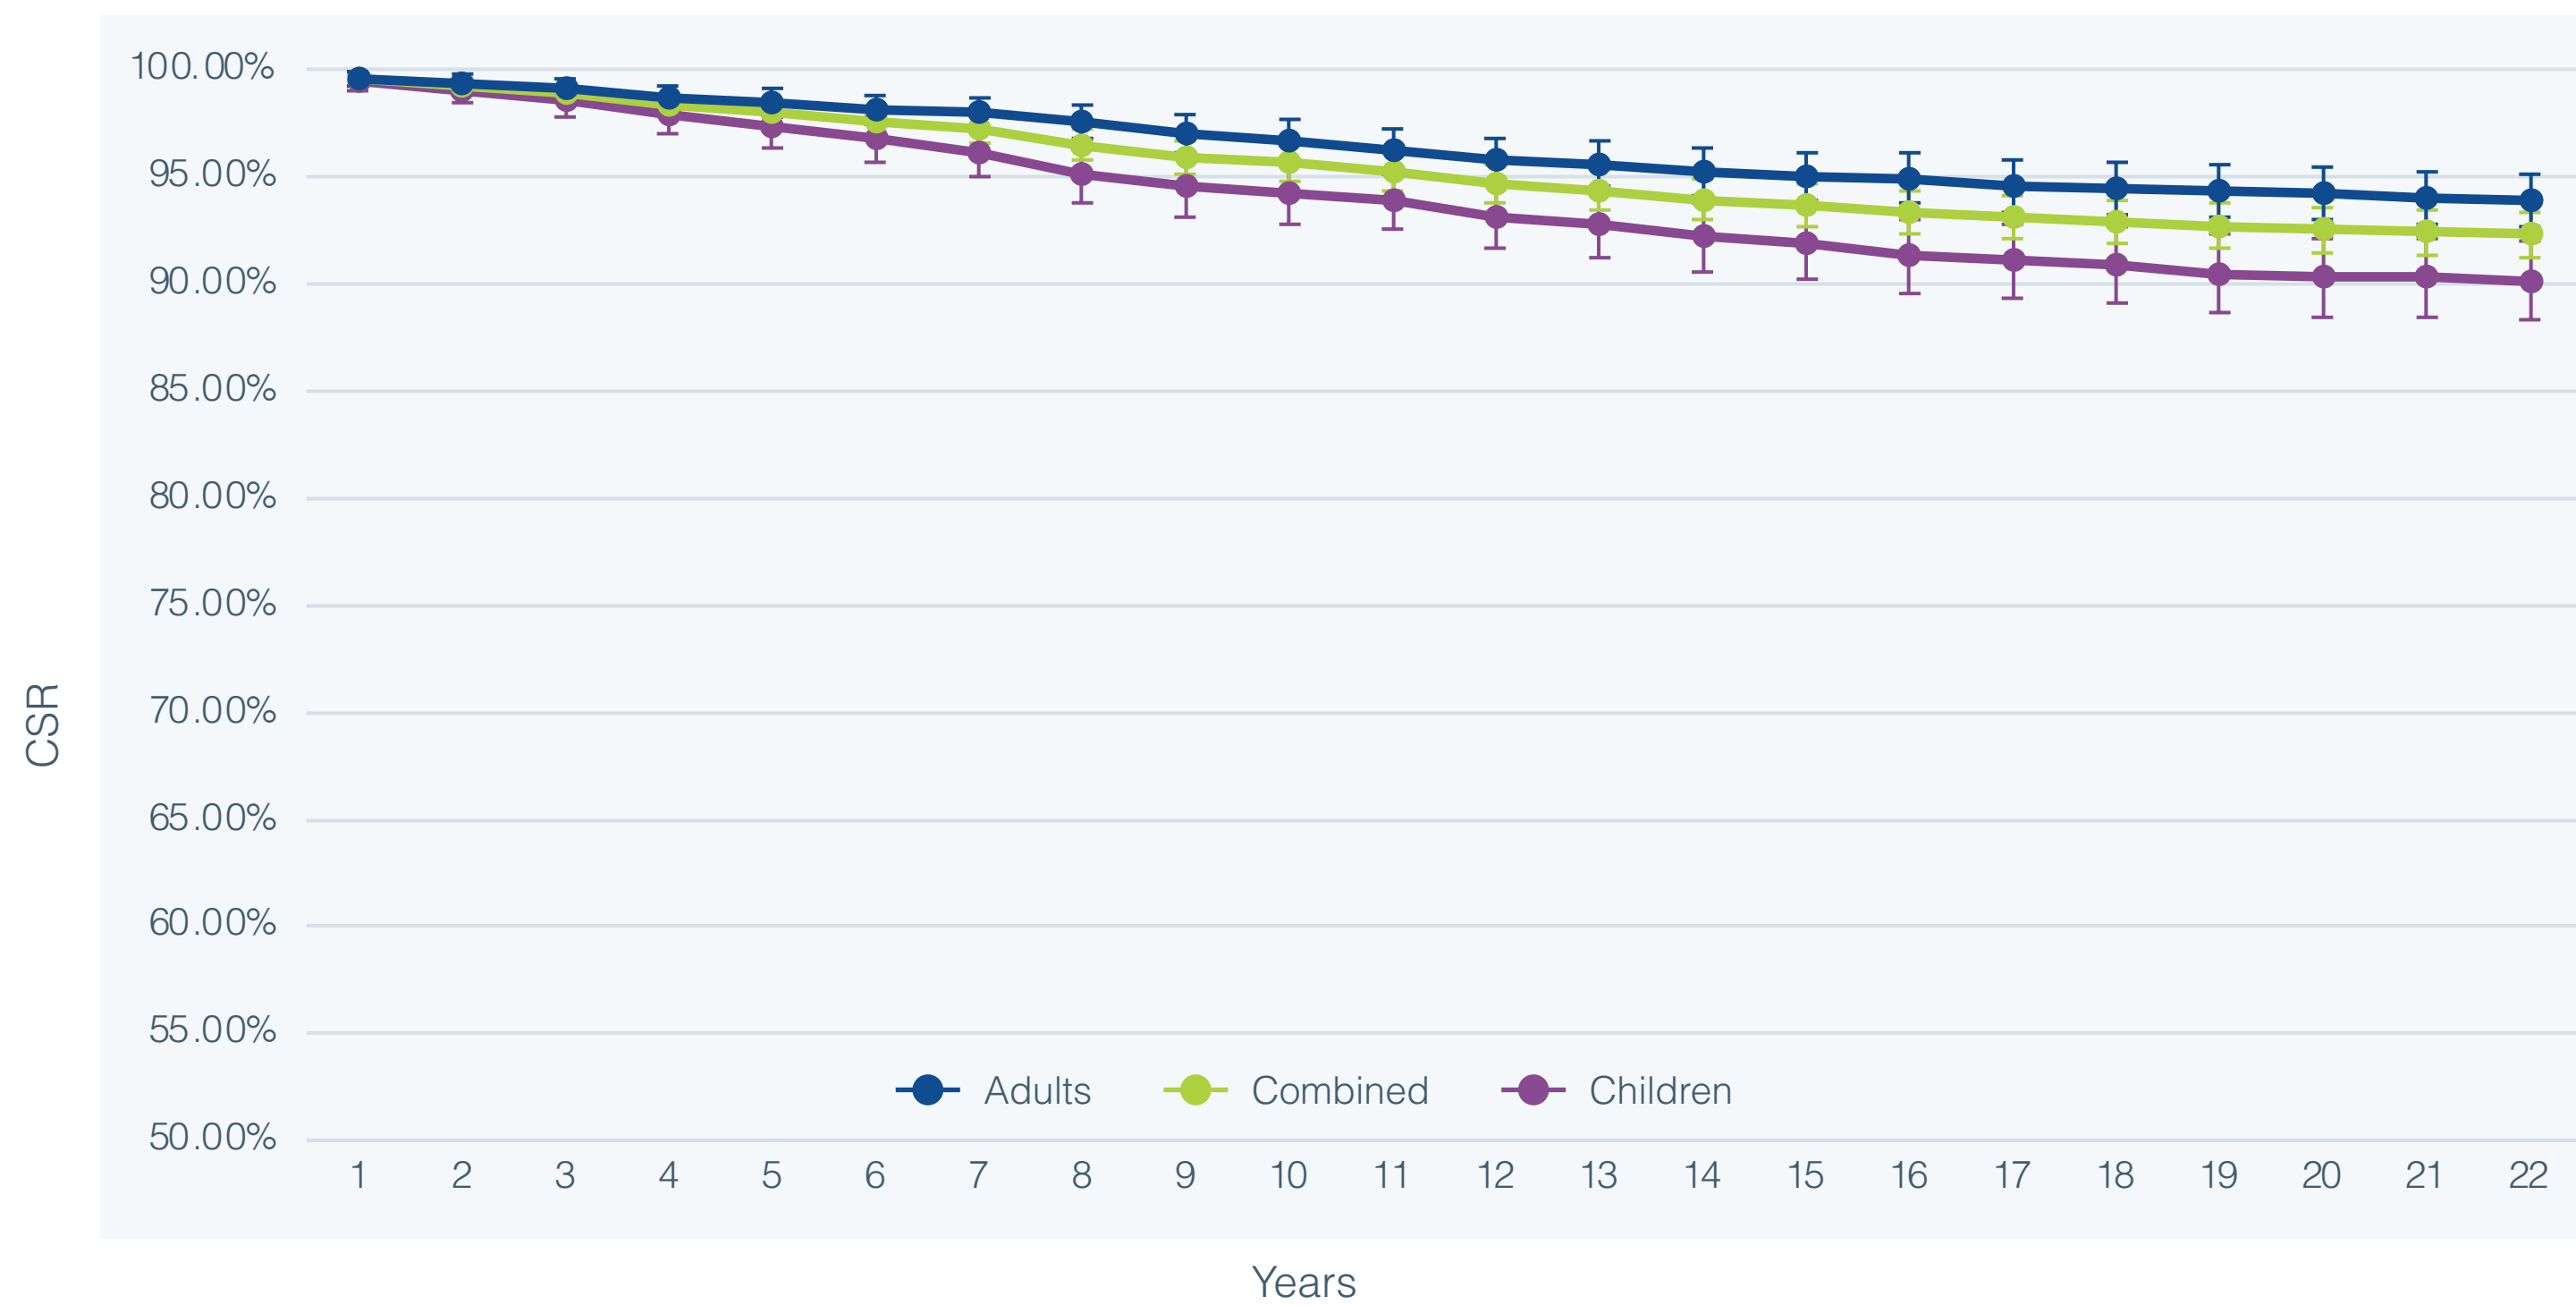

CUMULATIVE SURVIVAL RATE

Years in use	1	2	3	4	5	6	7	8	9	10	11
ADULTS	99.59%	99.31%	99.10%	98.60%	98.46%	98.10%	97.96%	97.52%	96.95%	96.66%	96.15%
COMBINED	99.53%	99.17%	98.85%	98.28%	97.96%	97.51%	97.18%	96.48%	95.90%	95.61%	95.20%
CHILDREN	99.45%	98.99%	98.52%	97.86%	97.29%	96.72%	96.15%	95.09%	94.51%	94.22%	93.92%

Years in use	12	13	14	15	16	17	18	19	20	21	22
ADULTS	95.72%	95.57%	95.21%	94.99%	94.92%	94.55%	94.40%	94.33%	94.18%	93.96%	93.86%
COMBINED	94.61%	94.36%	93.90%	93.65%	93.36%	93.06%	92.89%	92.68%	92.51%	92.38%	92.27%
CHILDREN	93.14%	92.75%	92.16%	91.86%	91.27%	91.07%	90.87%	90.47%	90.27%	90.27%	90.13%

ANSI/AAMI CI86

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

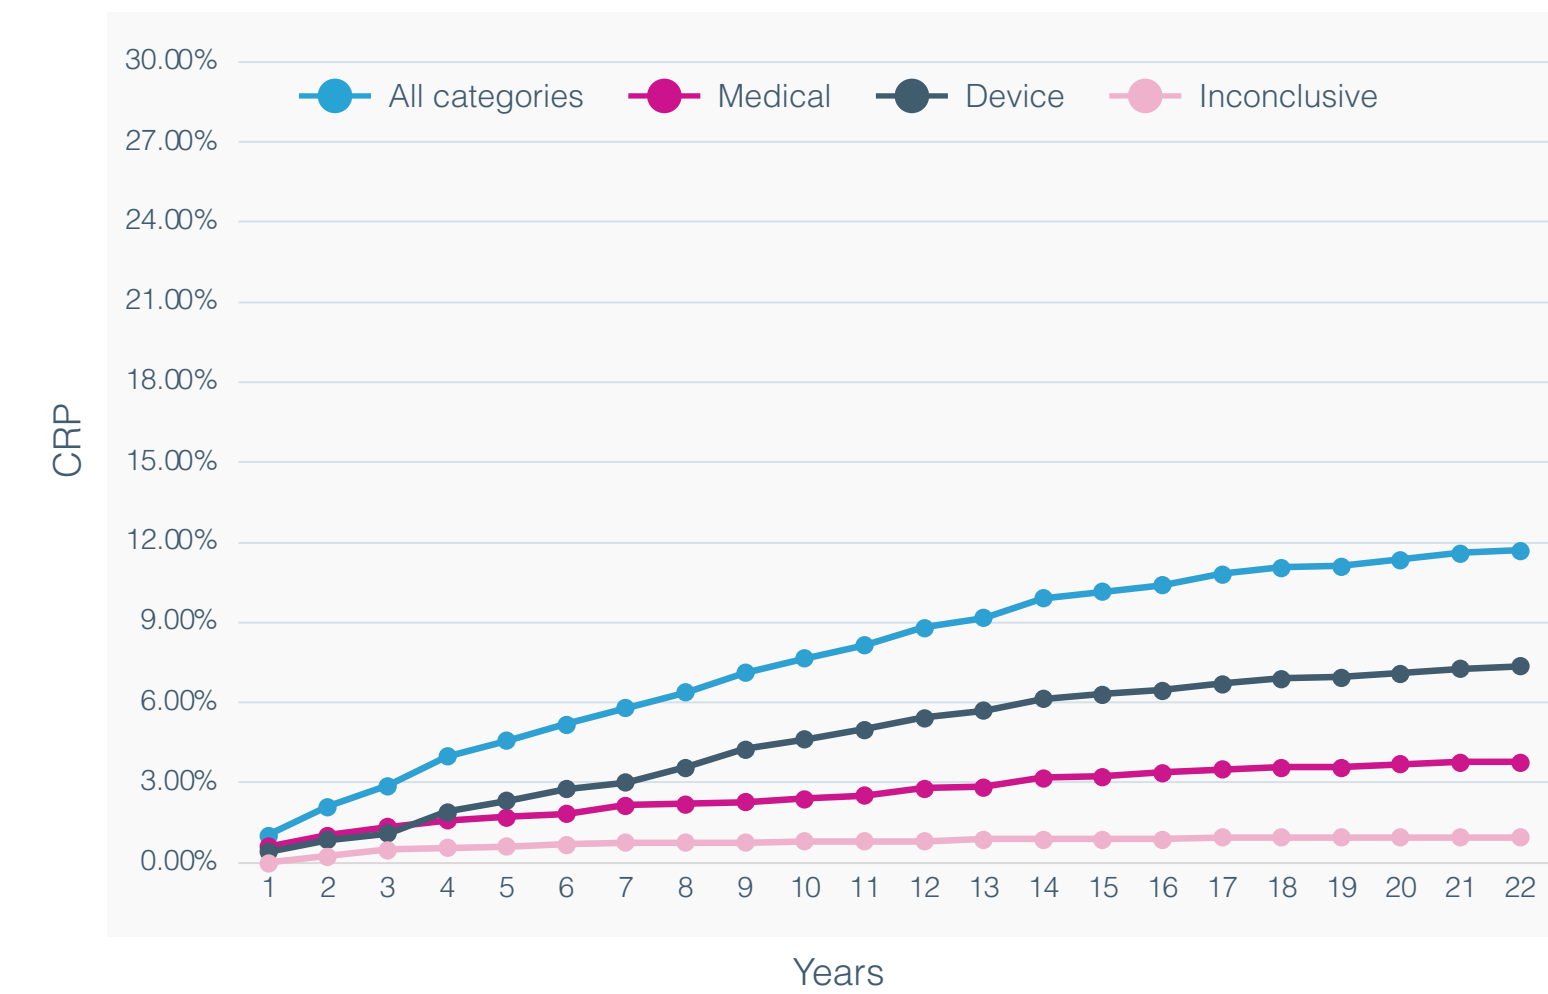

REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

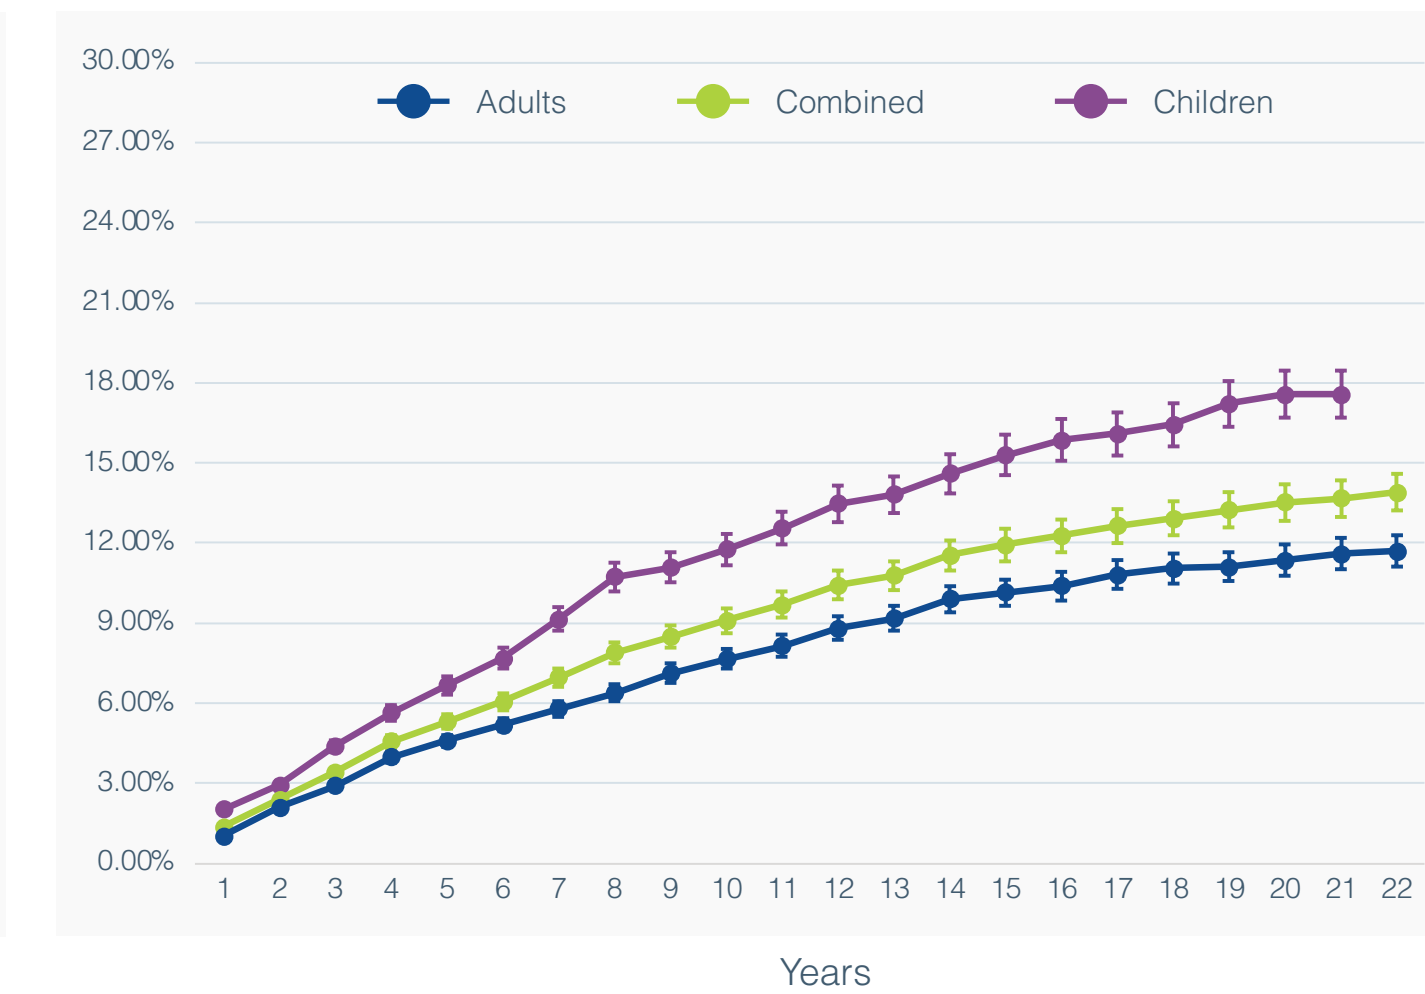

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

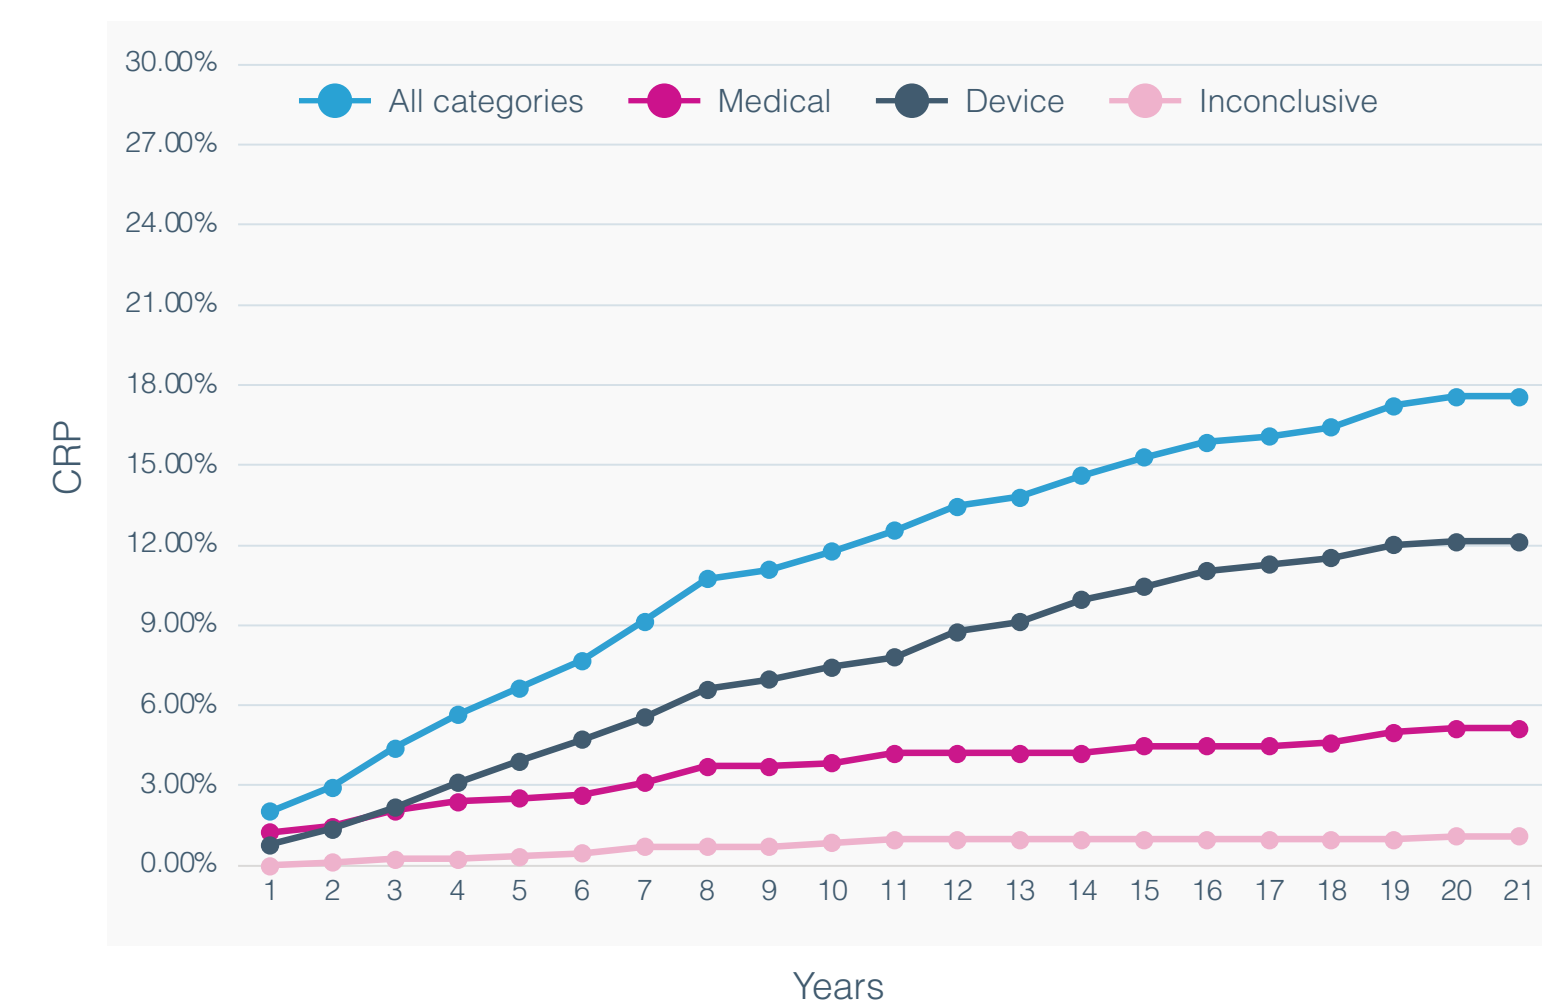

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

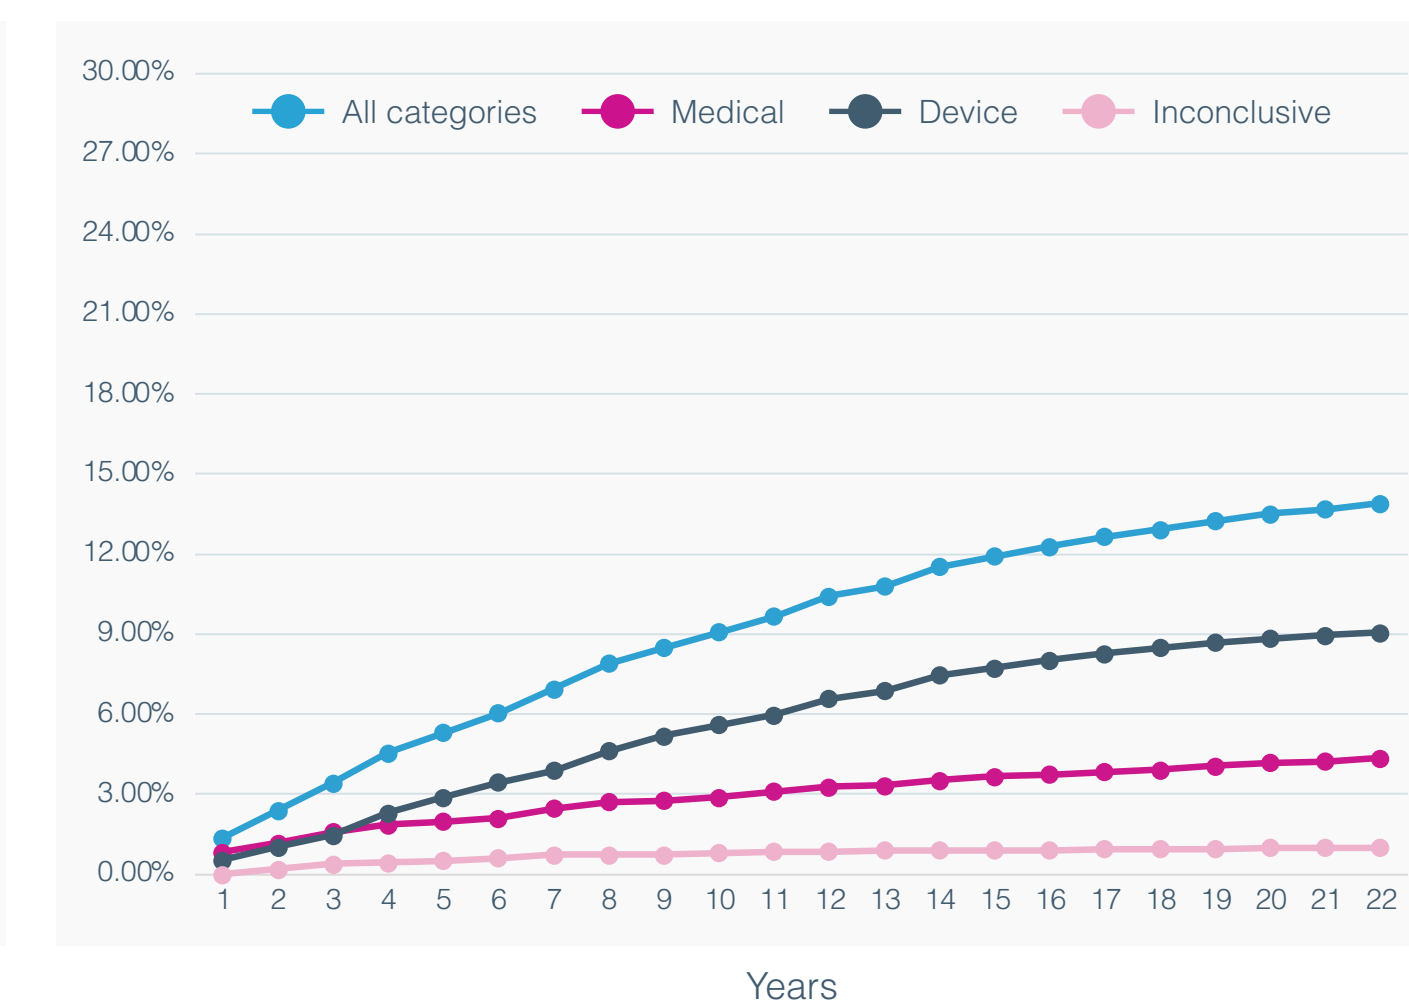

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	Total CI Lower
1	0.83%	0.55%	0.00%	1.37%	1.82%	0.92%
2	1.18%	1.03%	0.20%	2.39%	2.99%	1.80%
3	1.58%	1.47%	0.40%	3.42%	4.12%	2.71%
4	1.86%	2.31%	0.44%	4.56%	5.37%	3.75%
5	1.99%	2.88%	0.52%	5.31%	6.18%	4.44%
6	2.11%	3.44%	0.61%	6.06%	6.98%	5.13%
7	2.48%	3.89%	0.73%	6.96%	7.95%	5.97%
8	2.73%	4.62%	0.73%	7.91%	8.95%	6.86%
9	2.77%	5.19%	0.73%	8.50%	9.58%	7.41%
10	2.90%	5.60%	0.82%	9.09%	10.21%	7.97%
11	3.11%	5.97%	0.86%	9.68%	10.83%	8.53%
12	3.28%	6.59%	0.86%	10.43%	11.62%	9.24%
13	3.32%	6.88%	0.91%	10.79%	11.99%	9.58%
14	3.53%	7.46%	0.91%	11.54%	12.78%	10.29%
15	3.66%	7.75%	0.91%	11.93%	13.19%	10.67%
16	3.75%	8.04%	0.91%	12.29%	13.57%	11.01%
17	3.84%	8.29%	0.95%	12.65%	13.94%	11.35%
18	3.93%	8.49%	0.95%	12.92%	14.23%	11.62%
19	4.06%	8.70%	0.95%	13.24%	14.56%	11.92%
20	4.19%	8.83%	1.00%	13.52%	14.85%	12.19%
21	4.23%	8.96%	1.00%	13.68%	15.02%	12.34%
22	4.35%	9.07%	1.00%	13.89%	15.24%	12.54%

Please see the **Appendix** for a complete data set.

HIRES 90K vendor B

NUMBER OF REGISTERED HIRES 90K IMPLANTS (VENDOR B)

As of April 1, 2026.
Last year of distribution: subject to voluntary recall in 2006.[a]

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	2214	1849	4063[b]
ANSI/AAMI CI86	2558[c]	1505	4063

a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

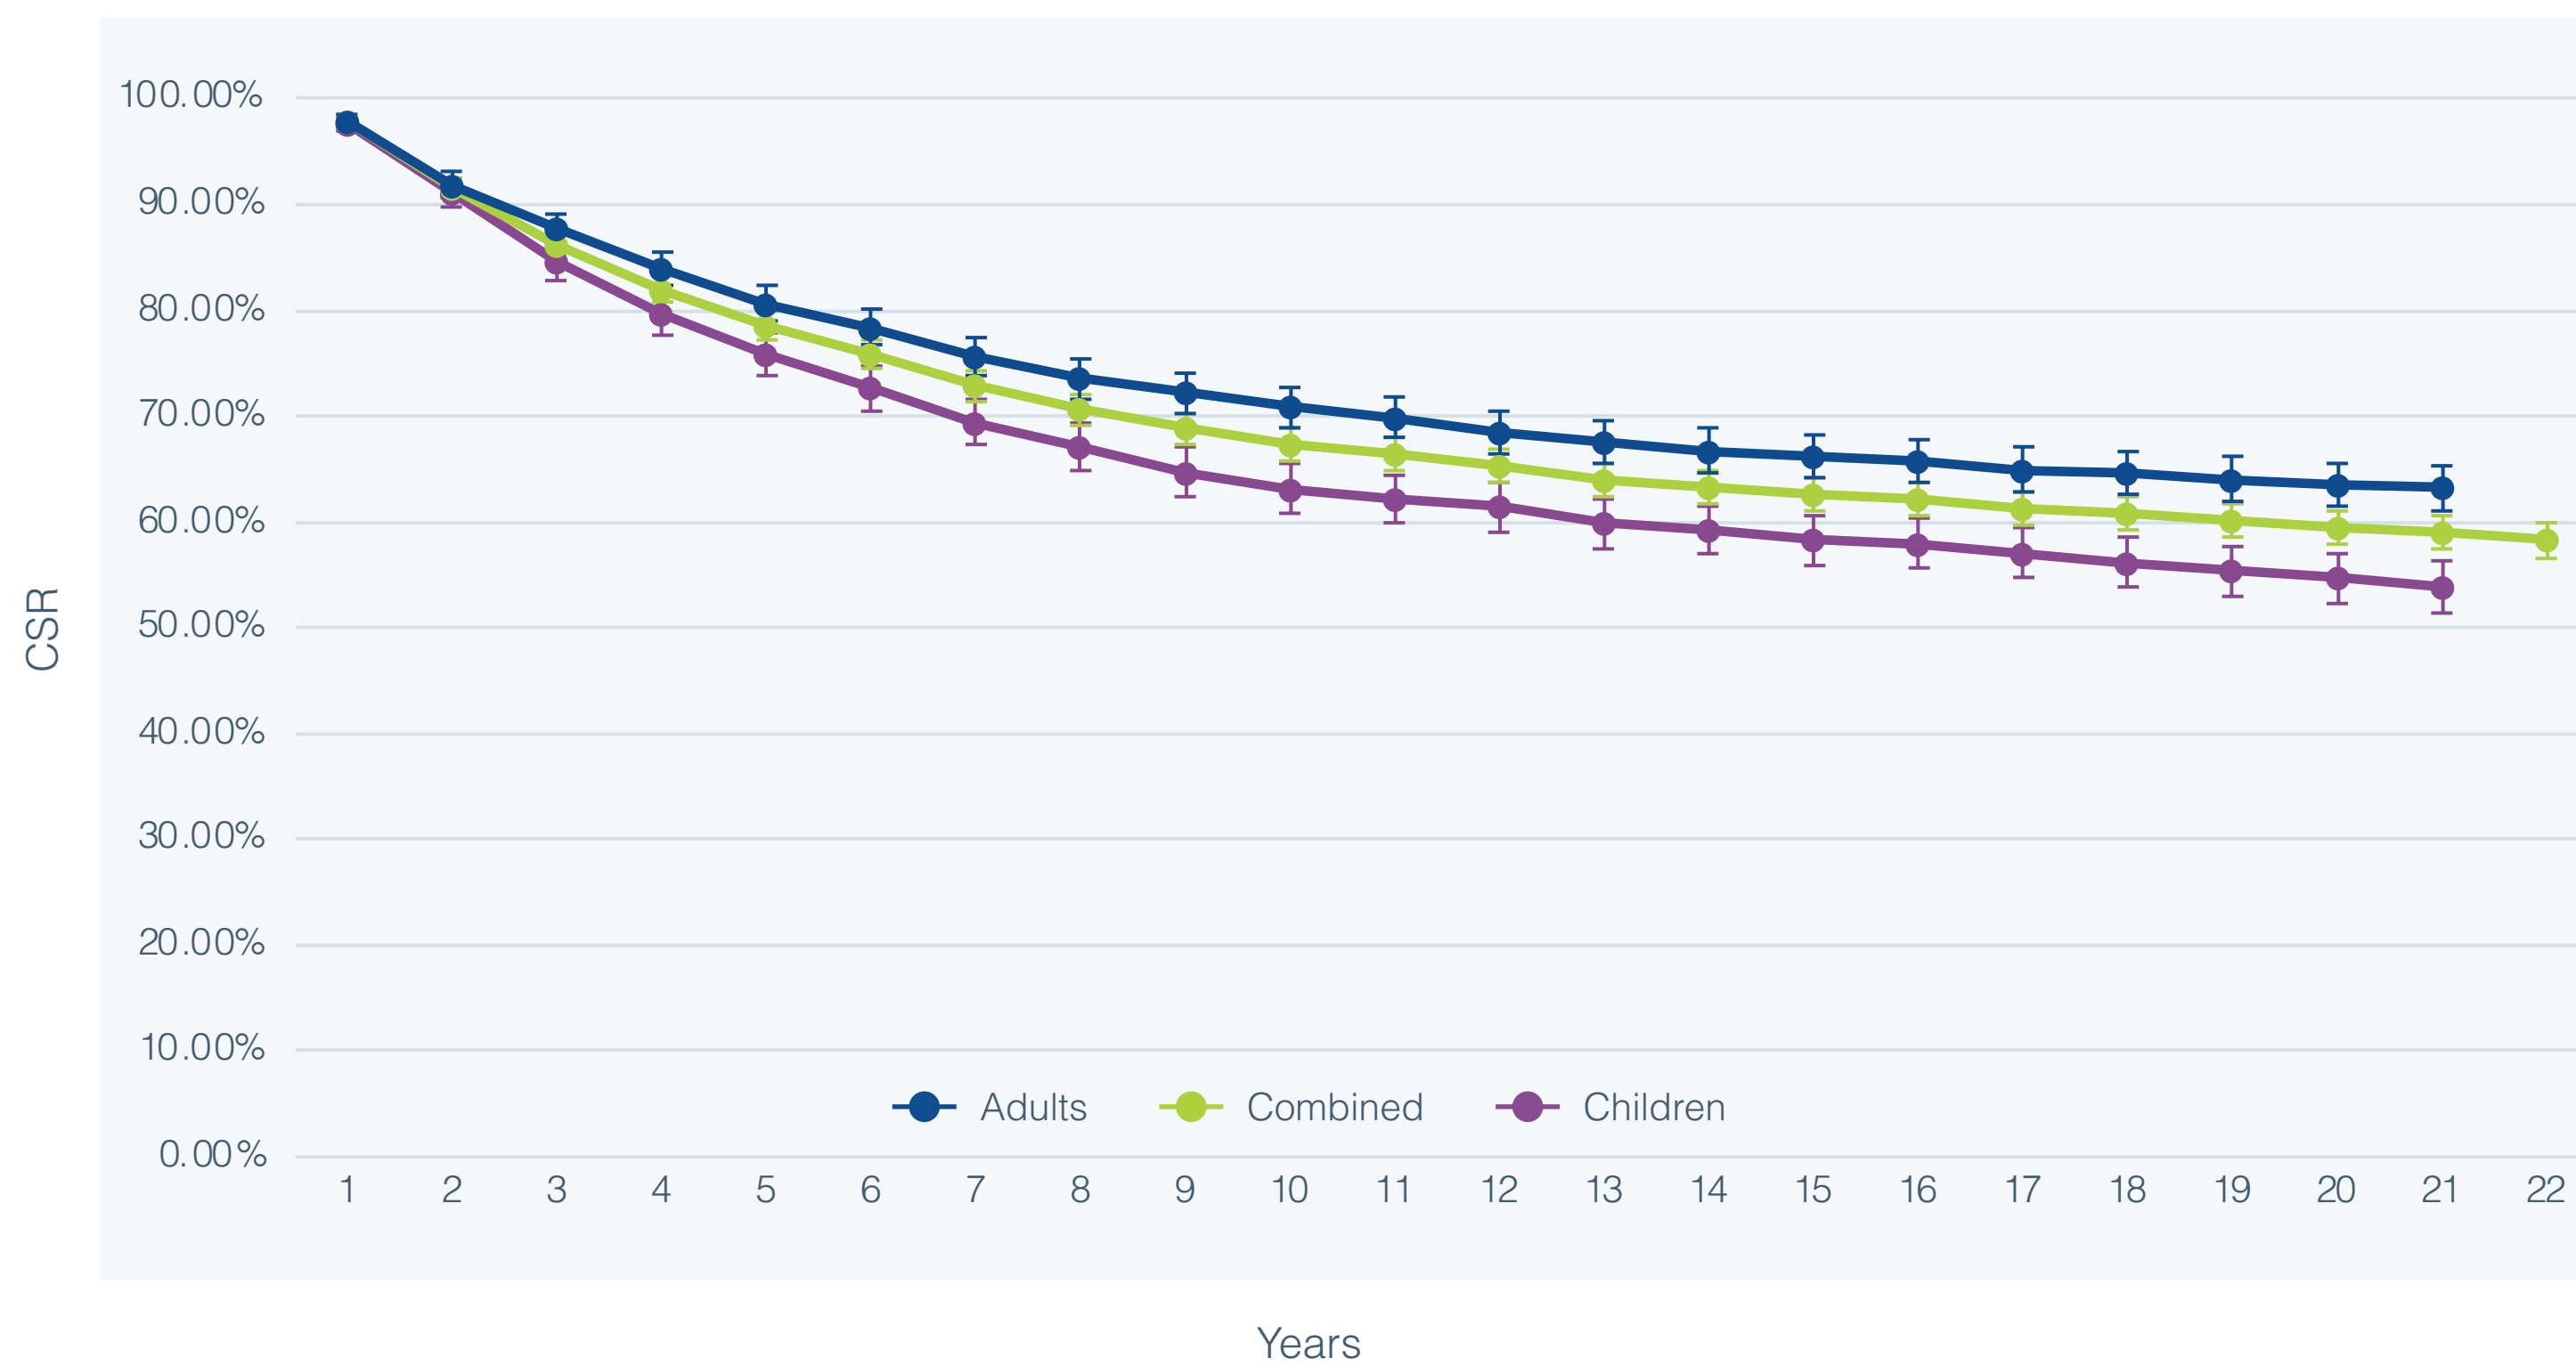

CUMULATIVE SURVIVAL RATE

Years in use	1	2	3	4	5	6	7	8	9	10	11
ADULTS	97.90%	91.91%	87.64%	83.88%	80.66%	78.41%	75.64%	73.57%	72.19%	70.81%	69.89%
COMBINED	97.79%	91.57%	86.25%	81.94%	78.48%	75.77%	72.83%	70.64%	68.80%	67.32%	66.39%
CHILDREN	97.65%	91.18%	84.60%	79.62%	75.87%	72.61%	69.45%	67.12%	64.73%	63.12%	62.19%

Years in use	12	13	14	15	16	17	18	19	20	21	22
ADULTS	68.50%	67.51%	66.73%	66.21%	65.69%	64.91%	64.59%	64.01%	63.49%	63.19%	N/A*
COMBINED	65.26%	64.01%	63.33%	62.62%	62.16%	61.32%	60.75%	60.08%	59.50%	58.93%	58.29%
CHILDREN	61.38%	59.80%	59.24%	58.29%	57.91%	57.01%	56.12%	55.35%	54.70%	53.78%	N/A*

*Sample size is not large enough for reporting.

ANSI/AAMI CI86

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

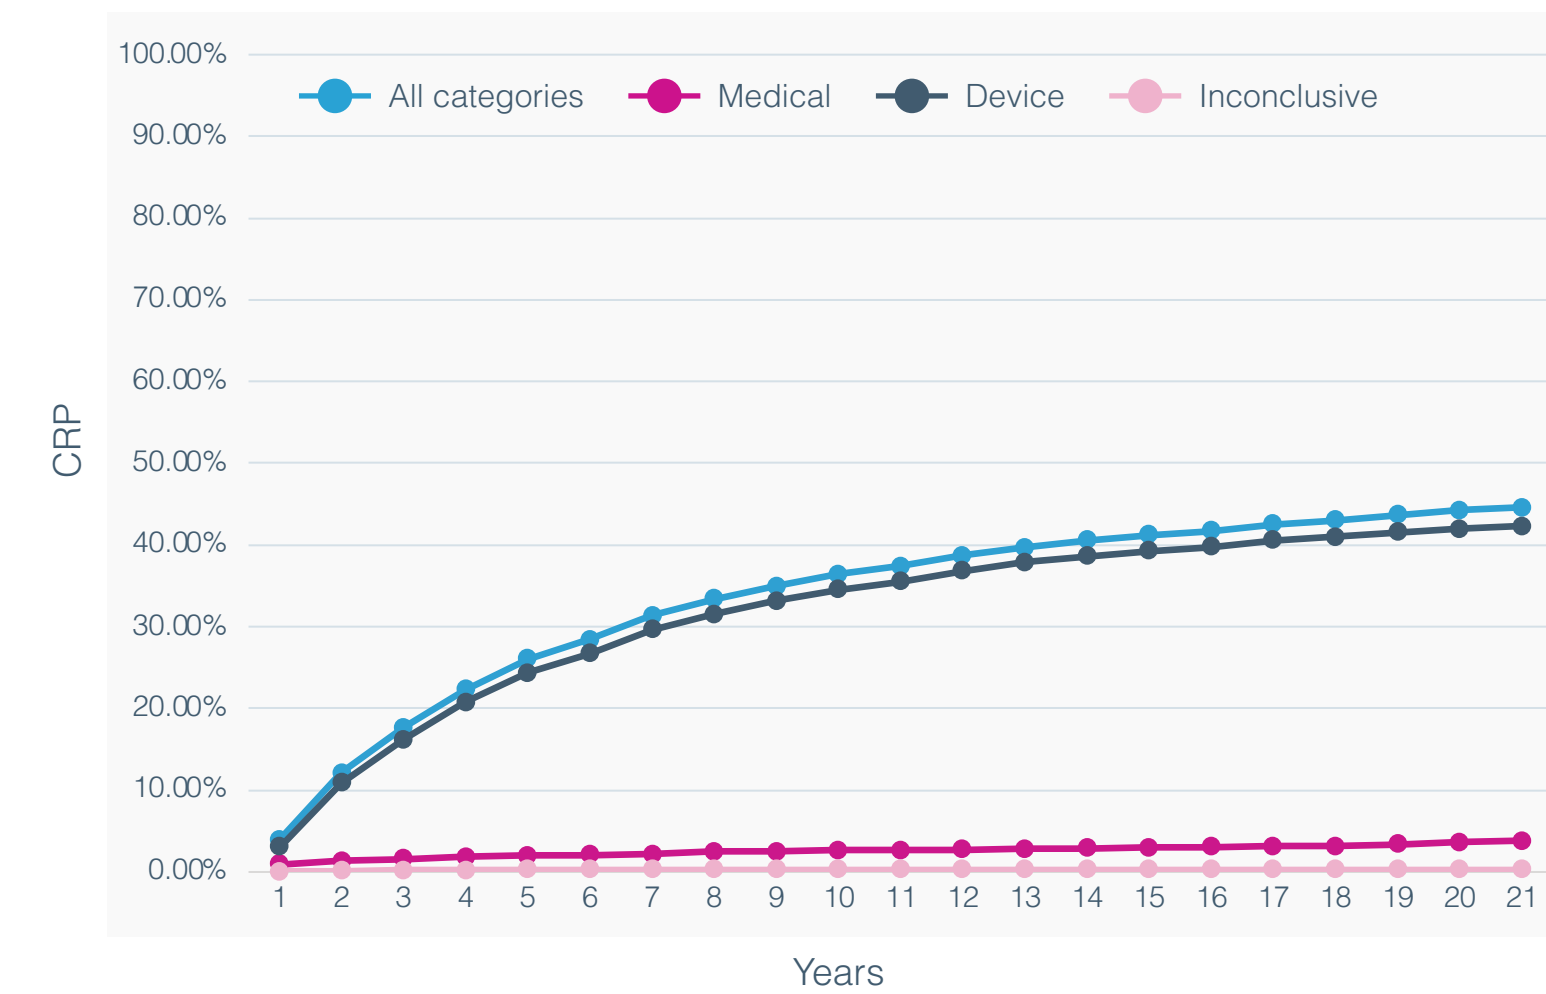

REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

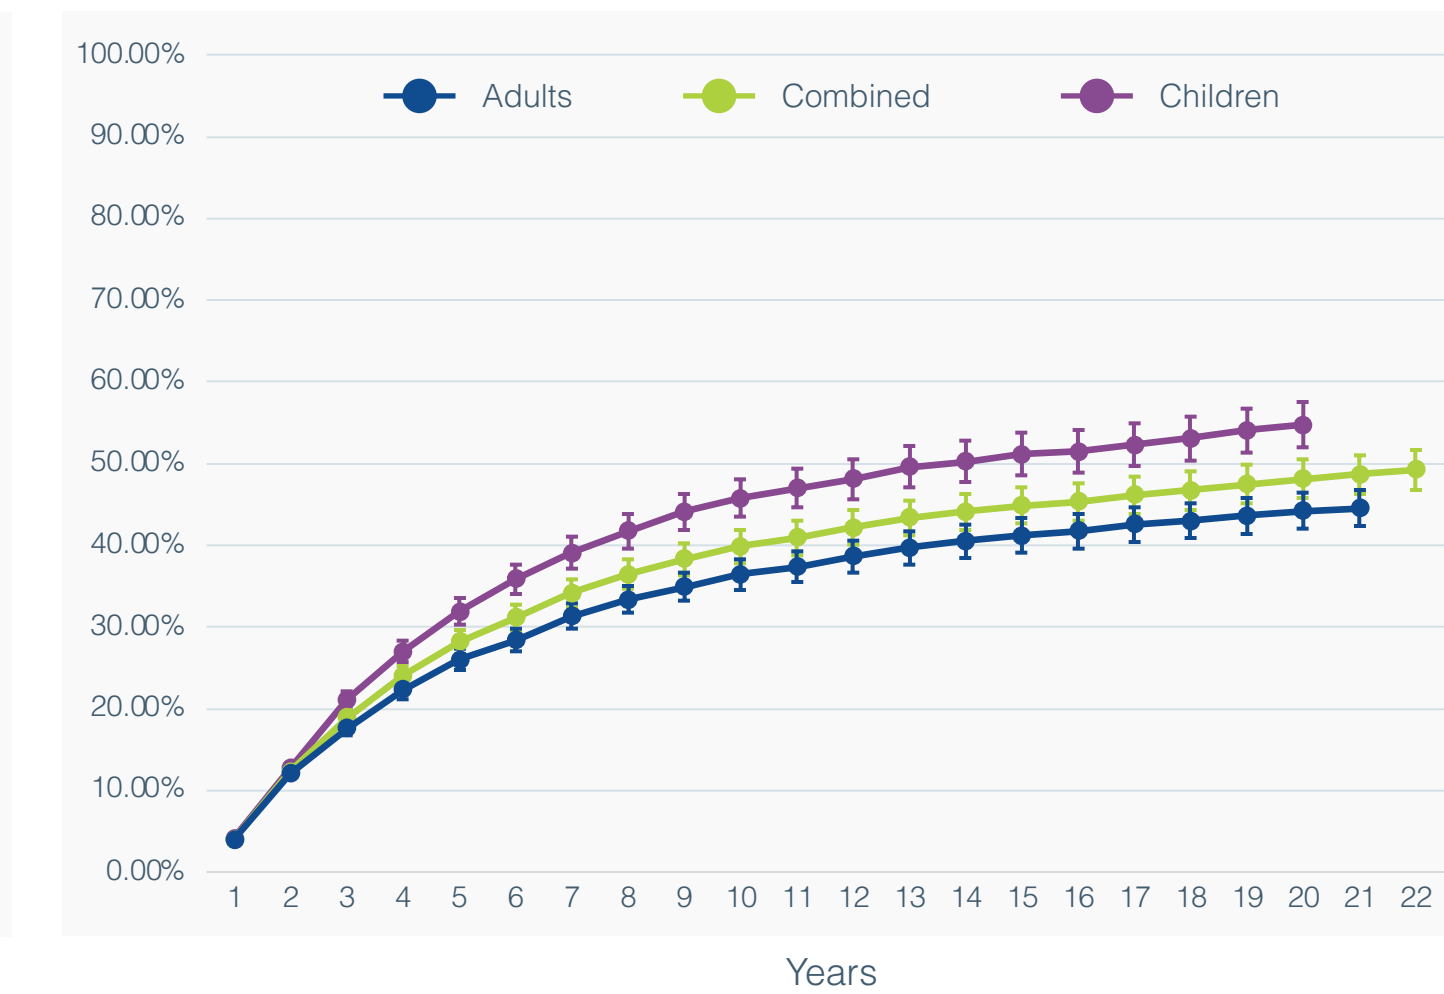

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

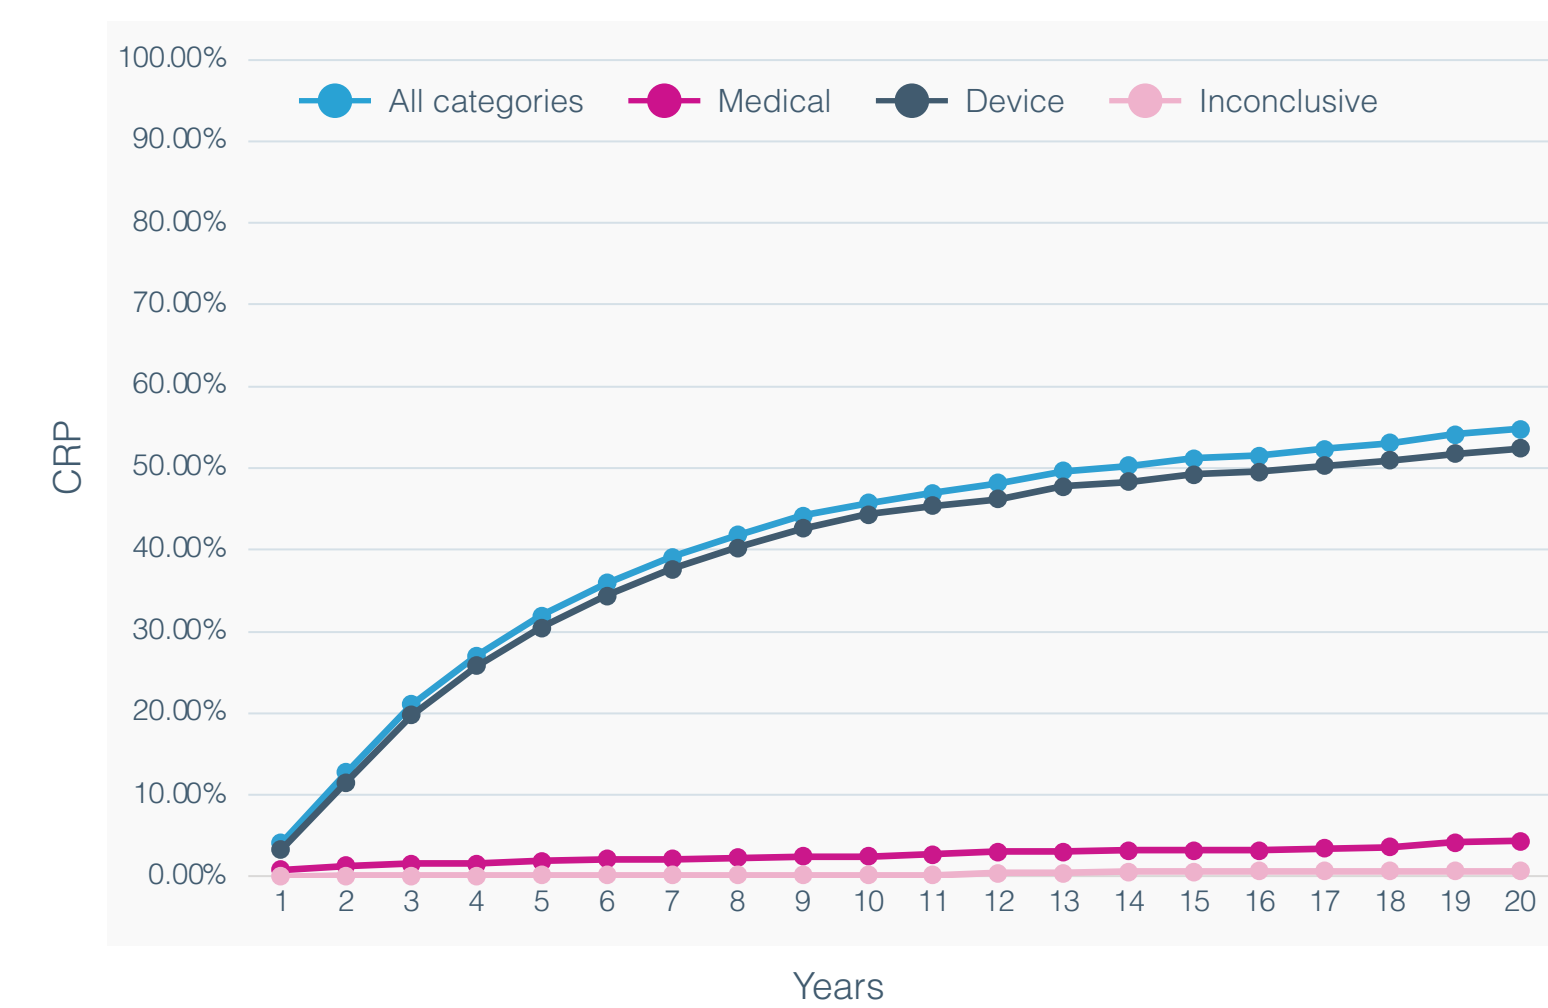

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

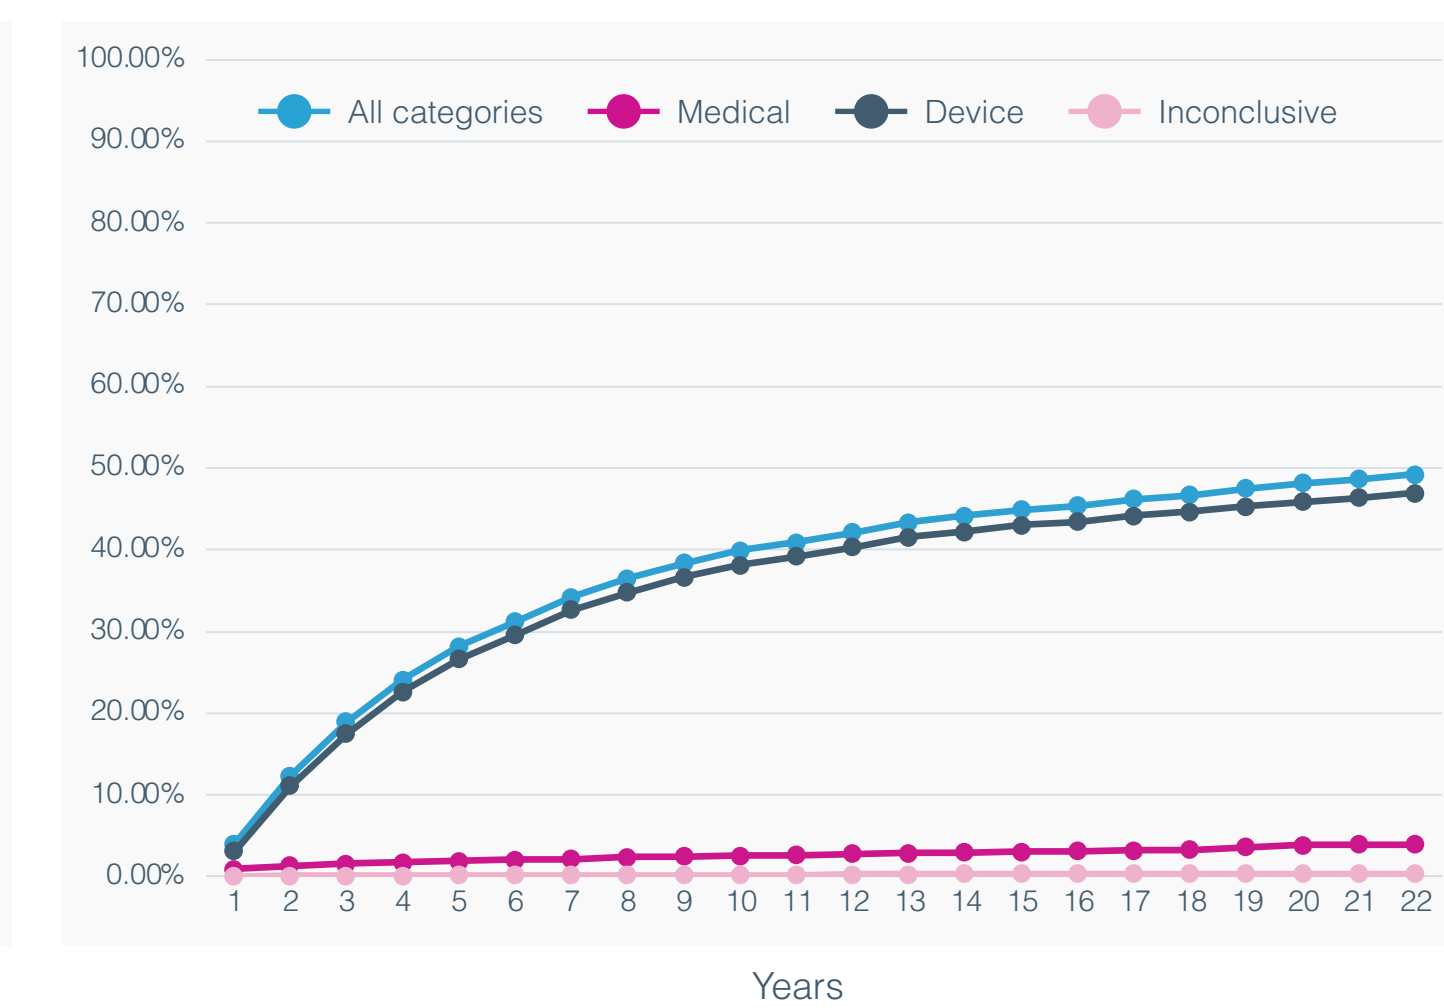

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	Total CI Lower
1	0.93%	3.12%	0.00%	4.02%	4.62%	3.41%
2	1.33%	11.09%	0.08%	12.34%	13.35%	11.33%
3	1.56%	17.52%	0.14%	18.92%	20.13%	17.72%
4	1.74%	22.61%	0.14%	24.06%	25.38%	22.75%
5	1.94%	26.62%	0.21%	28.20%	29.59%	26.81%
6	2.08%	29.56%	0.21%	31.16%	32.59%	29.74%
7	2.15%	32.62%	0.21%	34.21%	35.67%	32.74%
8	2.42%	34.77%	0.21%	36.48%	37.97%	34.99%
9	2.46%	36.65%	0.21%	38.33%	39.83%	36.83%
10	2.58%	38.16%	0.21%	39.88%	41.40%	38.37%
11	2.66%	39.17%	0.21%	40.91%	42.43%	39.39%
12	2.83%	40.31%	0.29%	42.16%	43.69%	40.64%
13	2.87%	41.53%	0.29%	43.37%	44.90%	41.84%
14	3.00%	42.23%	0.34%	44.15%	45.68%	42.61%
15	3.04%	42.98%	0.34%	44.90%	46.44%	43.37%
16	3.09%	43.40%	0.38%	45.36%	46.90%	43.82%
17	3.22%	44.16%	0.38%	46.17%	47.71%	44.62%
18	3.31%	44.68%	0.38%	46.72%	48.26%	45.18%
19	3.64%	45.31%	0.38%	47.50%	49.05%	45.96%
20	3.87%	45.84%	0.38%	48.14%	49.69%	46.59%
21	3.94%	46.36%	0.38%	48.67%	50.22%	47.12%
22	3.94%	46.95%	0.38%	49.23%	50.82%	47.64%

Please see the **Appendix** for a complete data set.

CII BIONIC EAR

The CII Bionic Ear cochlear implant is the base for the advanced technology found in Advanced Bionics implants today. The platform can still take advantage of the latest innovations today. It benefited from the mechanical improvement made to the earlier C1.2 implants.

NUMBER OF REGISTERED CII IMPLANTS

As of April 1, 2026.
Last year of distribution: 2004.[a]

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	3017	2094	5111[b]
ANSI/AAMI CI86	3393[c]	1718	5111

a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

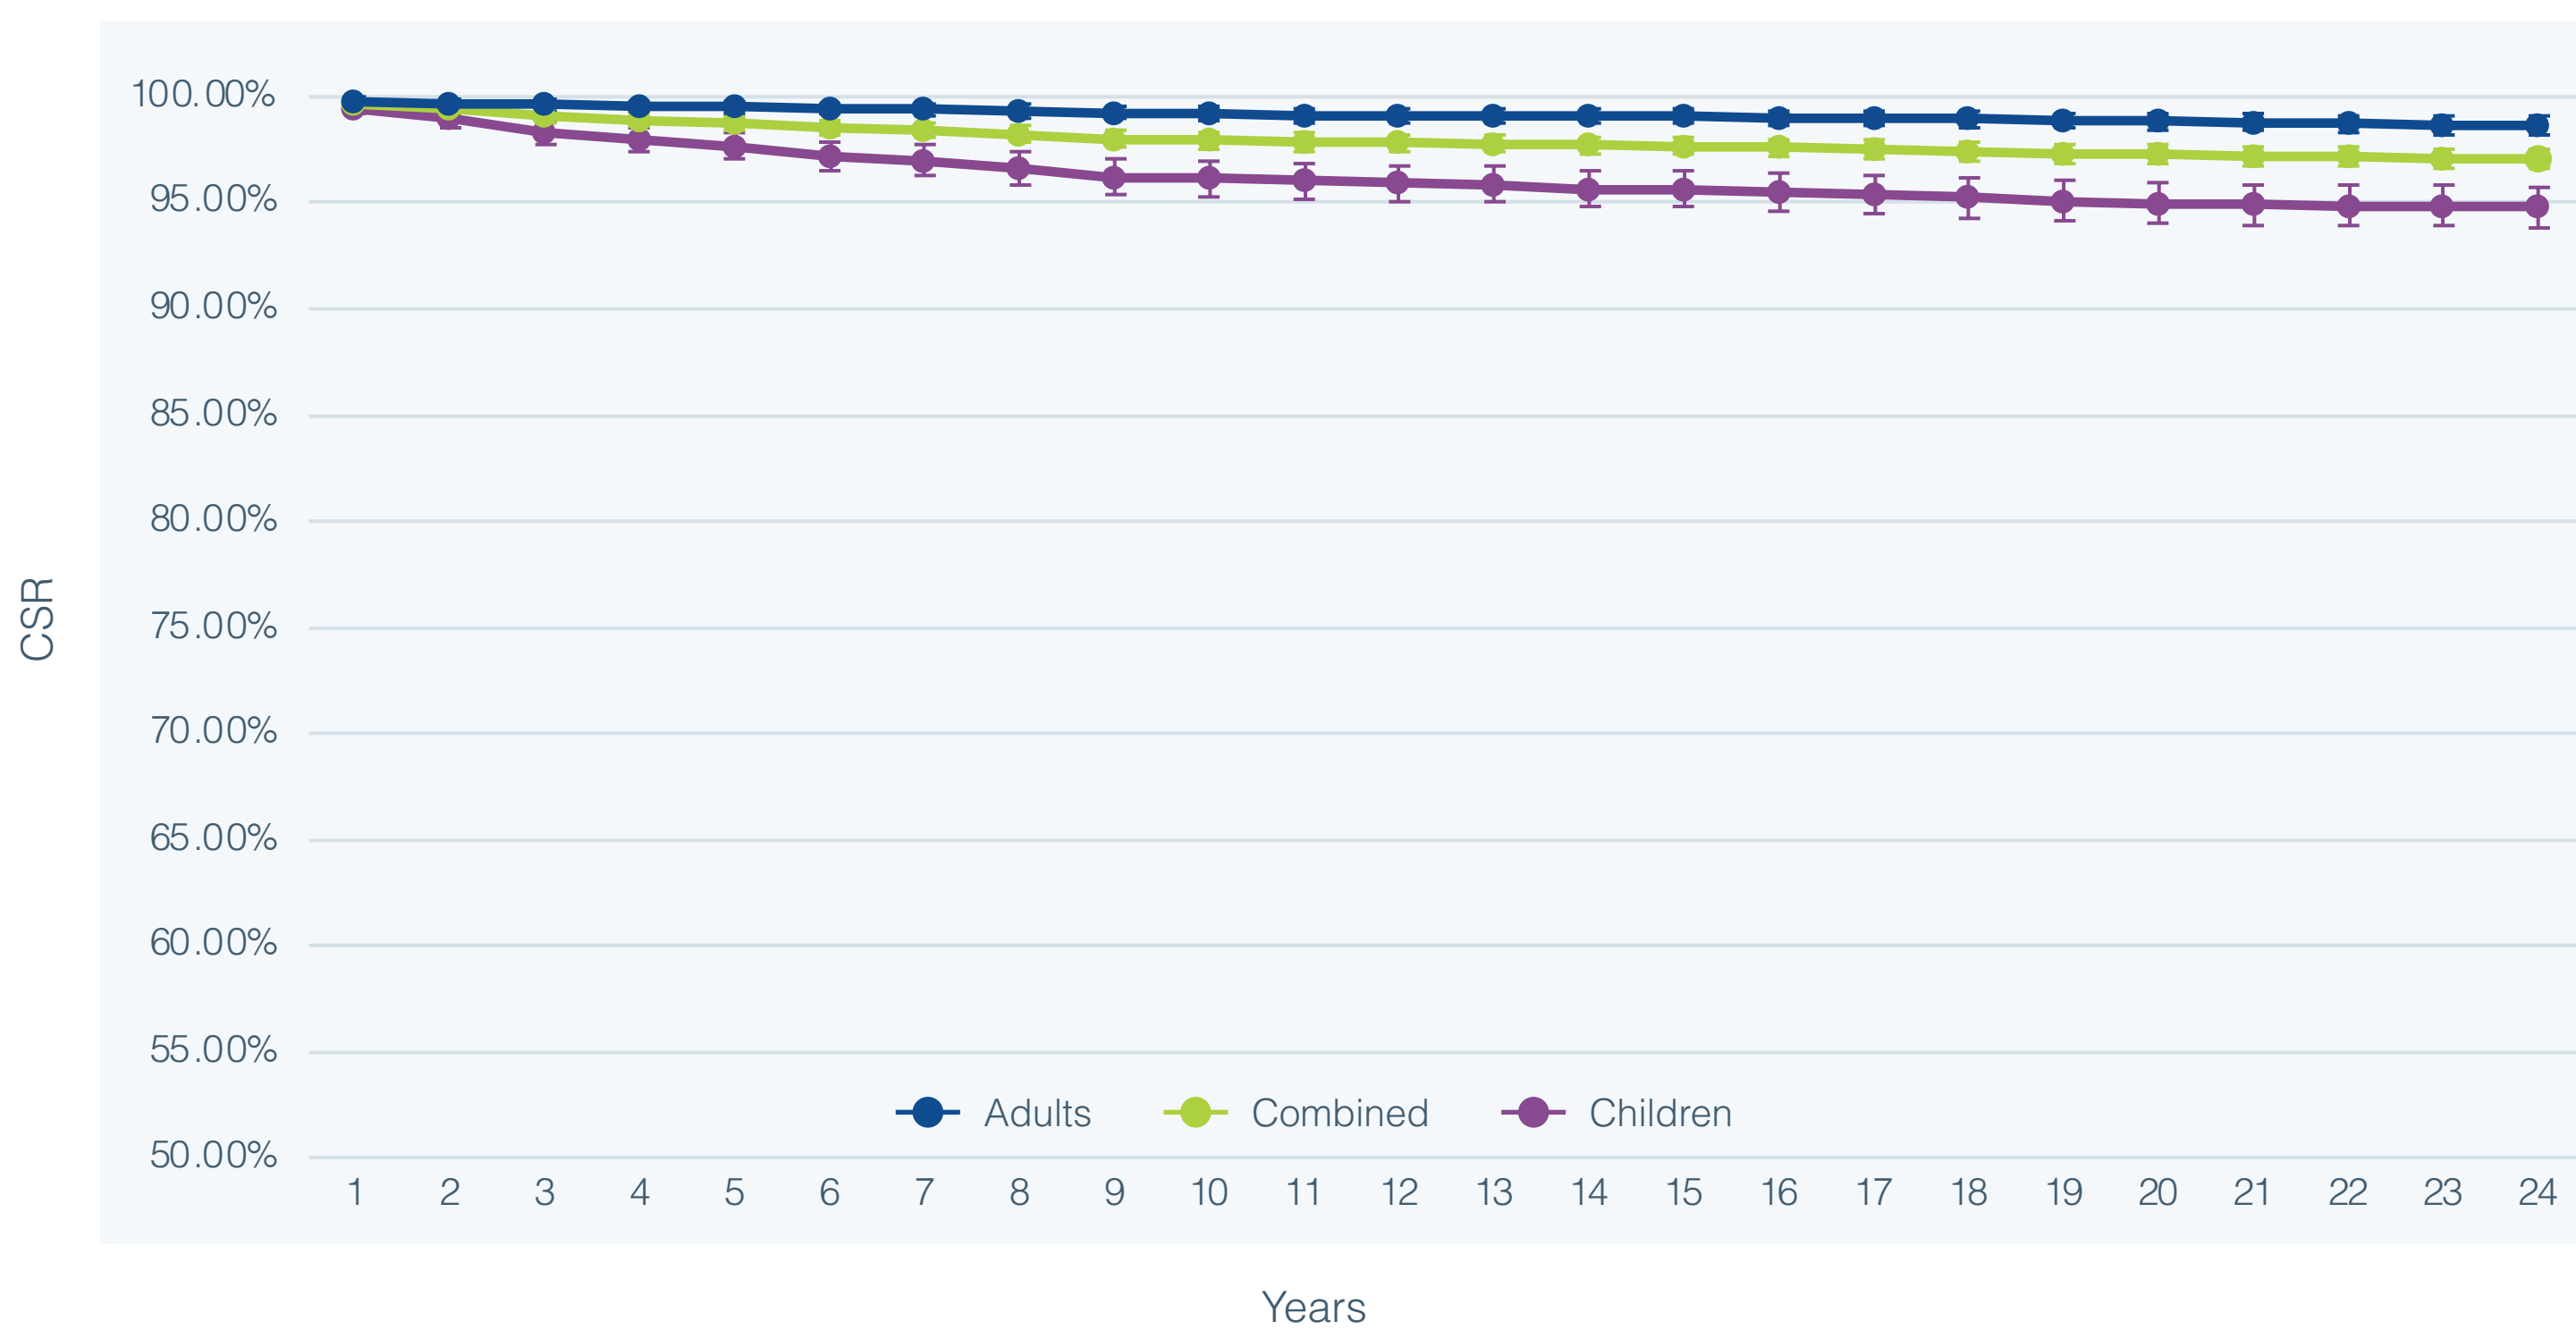

CUMULATIVE SURVIVAL RATE

Years in use	1	2	3	4	5	6	7	8	9	10	11	12
ADULTS	99.77%	99.70%	99.60%	99.53%	99.50%	99.43%	99.40%	99.33%	99.26%	99.22%	99.12%	99.12%
COMBINED	99.65%	99.41%	99.07%	98.89%	98.75%	98.51%	98.41%	98.23%	98.02%	97.96%	97.86%	97.82%
CHILDREN	99.47%	98.99%	98.31%	97.97%	97.67%	97.18%	96.98%	96.63%	96.22%	96.12%	96.02%	95.92%

Years in use	13	14	15	16	17	18	19	20	21	22	23	24
ADULTS	99.12%	99.09%	99.05%	99.02%	98.98%	98.95%	98.88%	98.84%	98.77%	98.70%	98.63%	98.63%
COMBINED	97.80%	97.69%	97.67%	97.59%	97.53%	97.44%	97.34%	97.28%	97.21%	97.15%	97.10%	97.07%
CHILDREN	95.87%	95.66%	95.66%	95.51%	95.40%	95.25%	95.09%	94.99%	94.93%	94.88%	94.88%	94.79%

ANSI/AAMI CI86

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

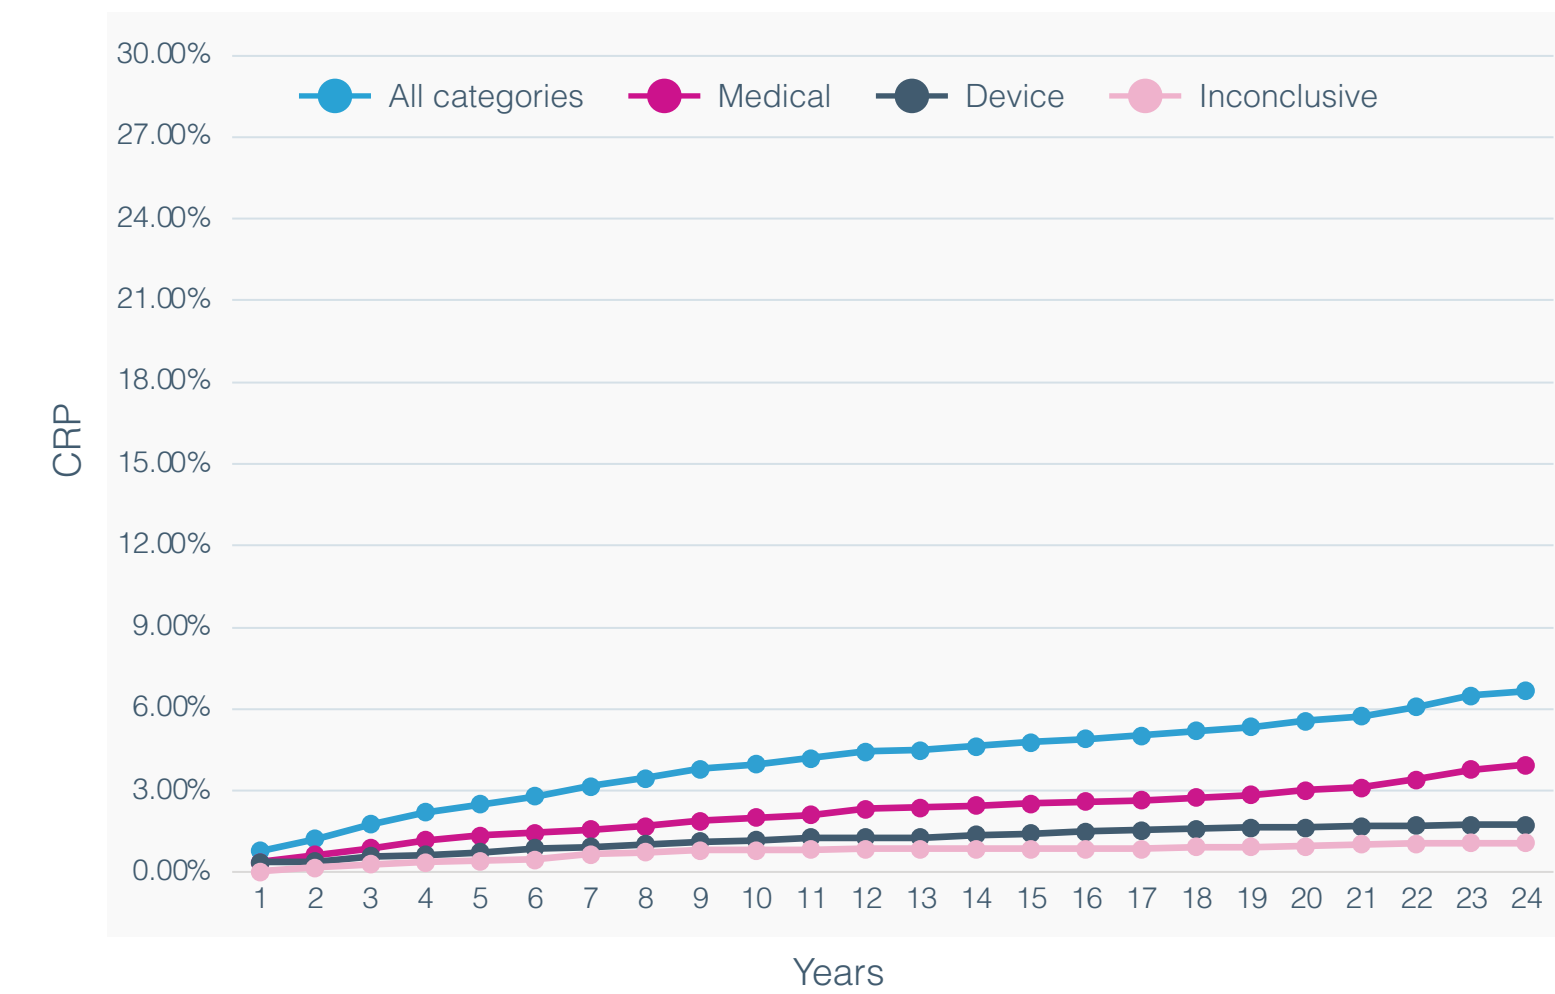

REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

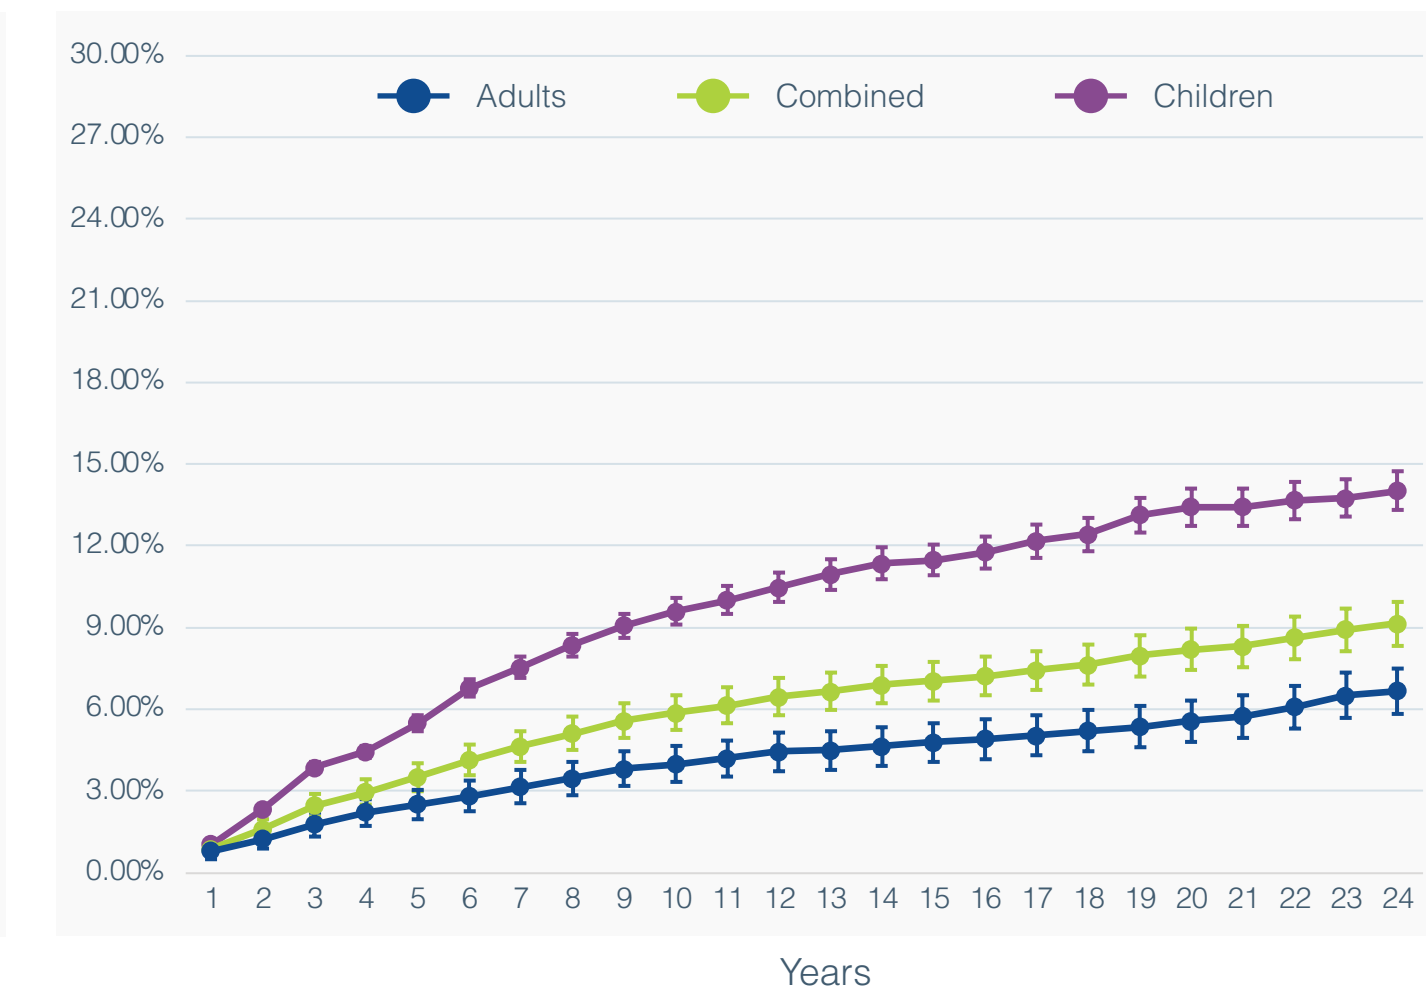

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

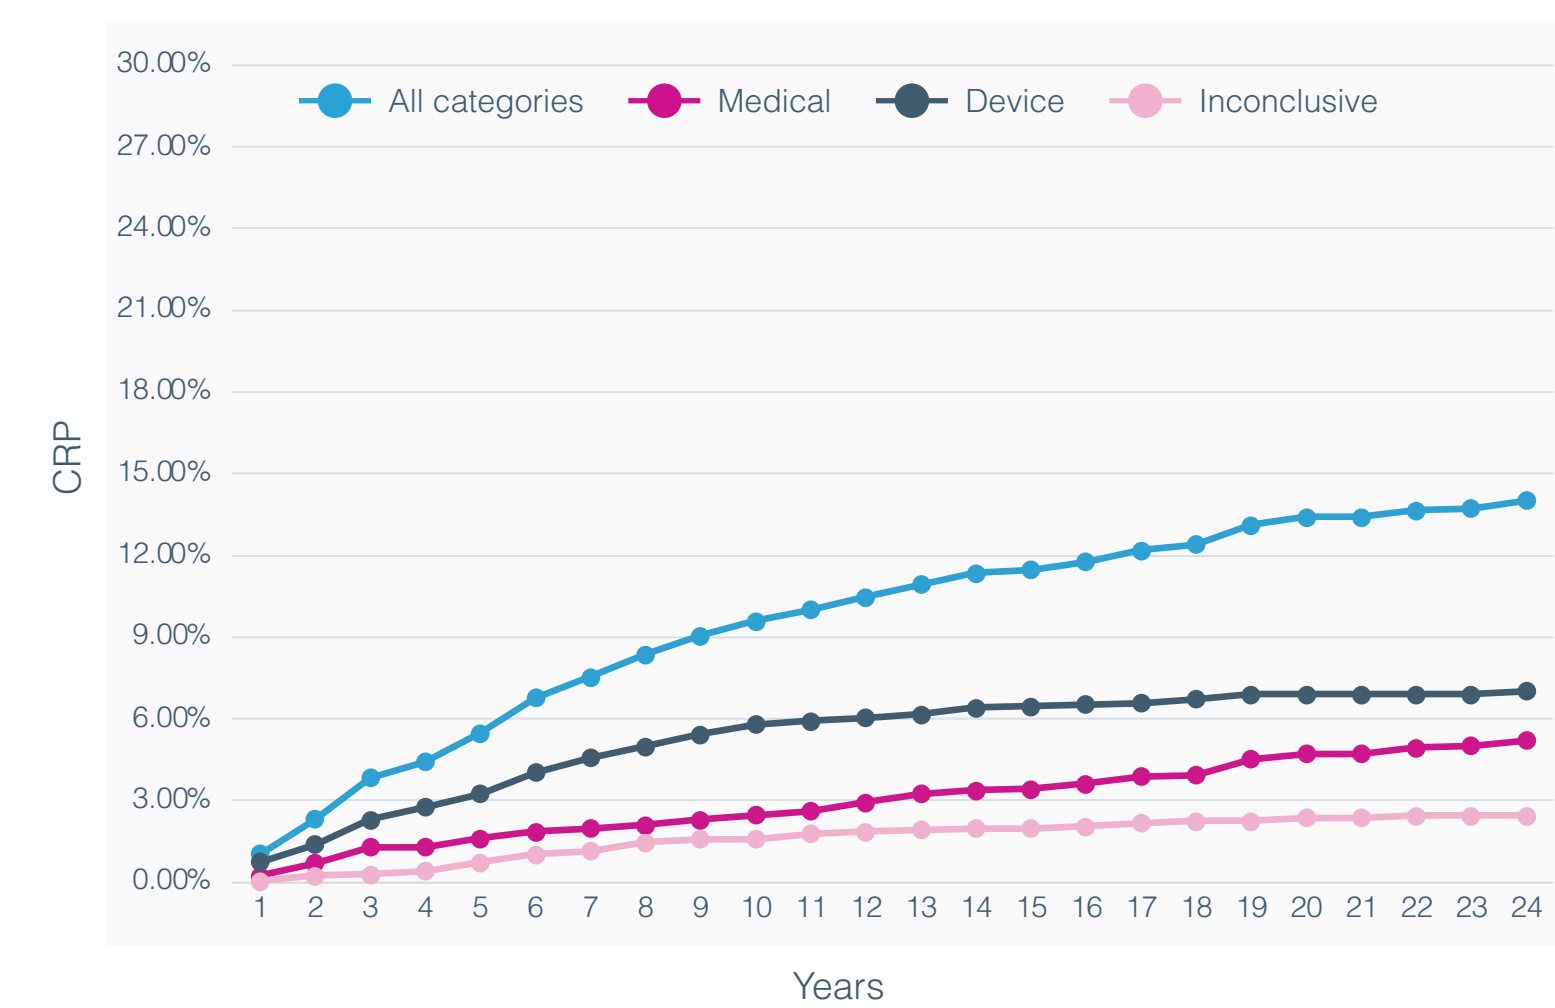

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

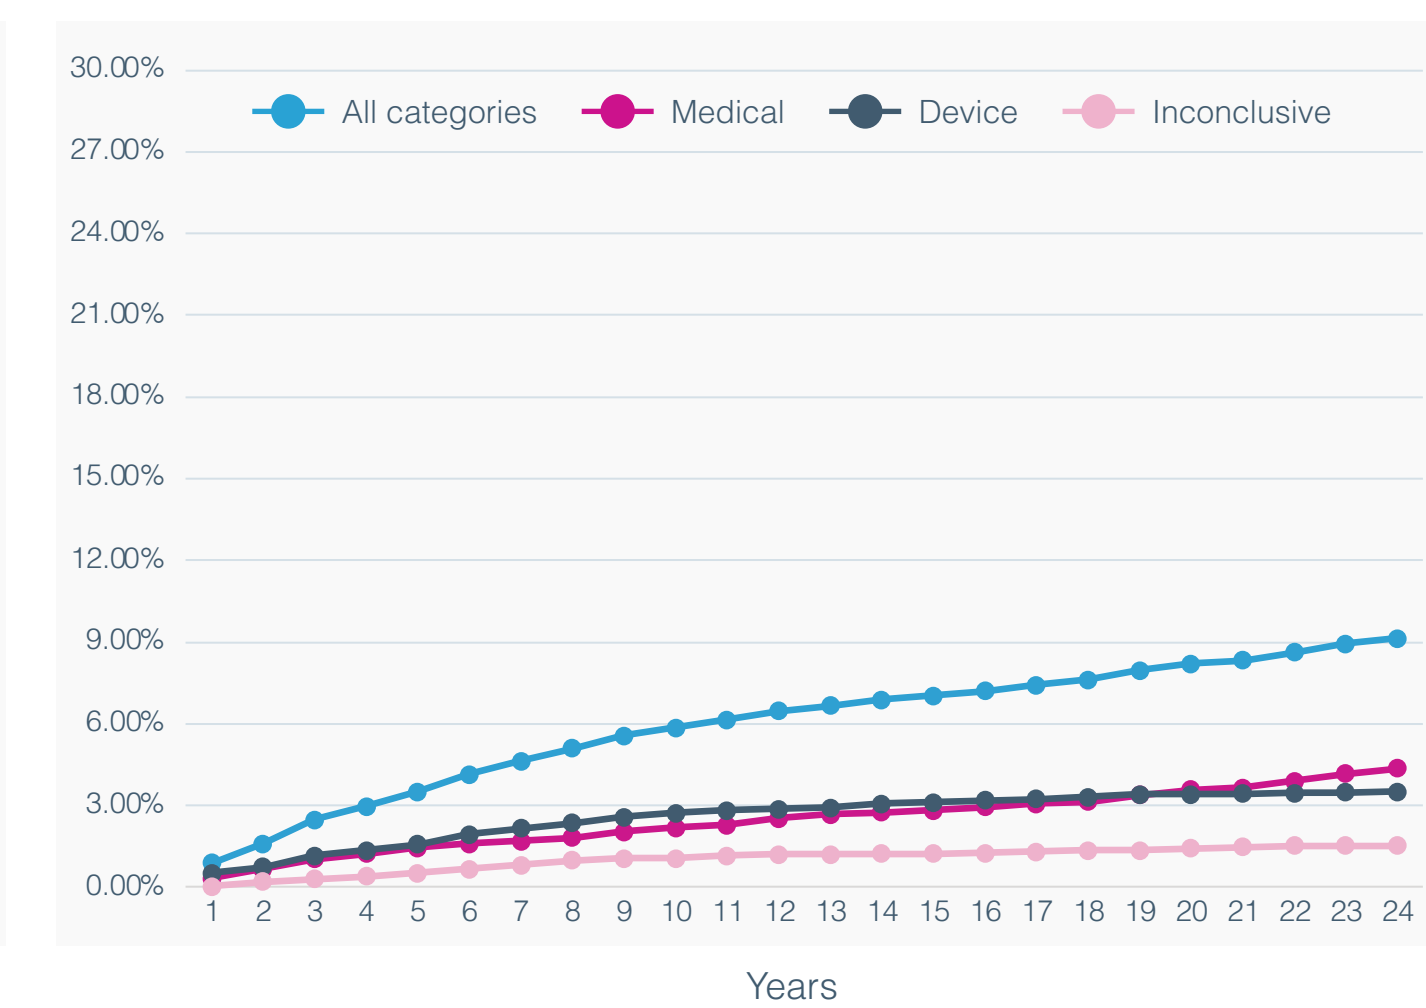

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	Total CI Lower
1	0.33%	0.51%	0.04%	0.88%	1.14%	0.62%
2	0.67%	0.75%	0.20%	1.61%	1.95%	1.26%
3	1.03%	1.16%	0.30%	2.47%	2.89%	2.04%
4	1.23%	1.36%	0.40%	2.96%	3.42%	2.49%
5	1.45%	1.58%	0.52%	3.51%	4.01%	3.00%
6	1.59%	1.94%	0.66%	4.14%	4.68%	3.59%
7	1.71%	2.16%	0.82%	4.63%	5.21%	4.05%
8	1.83%	2.37%	0.99%	5.10%	5.71%	4.50%
9	2.03%	2.57%	1.07%	5.57%	6.20%	4.94%
10	2.18%	2.73%	1.07%	5.87%	6.52%	5.22%
11	2.28%	2.83%	1.15%	6.15%	6.80%	5.49%
12	2.53%	2.88%	1.20%	6.46%	7.14%	5.79%
13	2.67%	2.92%	1.22%	6.66%	7.34%	5.97%
14	2.75%	3.06%	1.24%	6.89%	7.59%	6.20%
15	2.83%	3.12%	1.24%	7.03%	7.73%	6.33%
16	2.94%	3.18%	1.26%	7.21%	7.92%	6.50%
17	3.06%	3.25%	1.30%	7.43%	8.15%	6.71%
18	3.14%	3.31%	1.36%	7.62%	8.35%	6.90%
19	3.39%	3.41%	1.36%	7.96%	8.71%	7.22%
20	3.58%	3.41%	1.43%	8.20%	8.95%	7.45%
21	3.64%	3.43%	1.47%	8.32%	9.08%	7.56%
22	3.90%	3.45%	1.51%	8.62%	9.39%	7.85%
23	4.18%	3.48%	1.54%	8.93%	9.72%	8.14%
24	4.37%	3.51%	1.54%	9.14%	9.94%	8.34%

Please see the **Appendix** for a complete data set.

CLARION 1.2

The Clarion 1.2 (C1.2) implant offers mechanical improvements over its predecessor the C1.0 implant, which first introduced independent current-sources, a key technology differentiator for Advanced Bionics implants.

NUMBER OF REGISTERED C1.2 IMPLANTS

As of April 1, 2026.
Last year of distribution: 2004.[a]

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	4355	4159	8514[b]
ANSI/AAMI CI86	4988[c]	3526	8514

a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

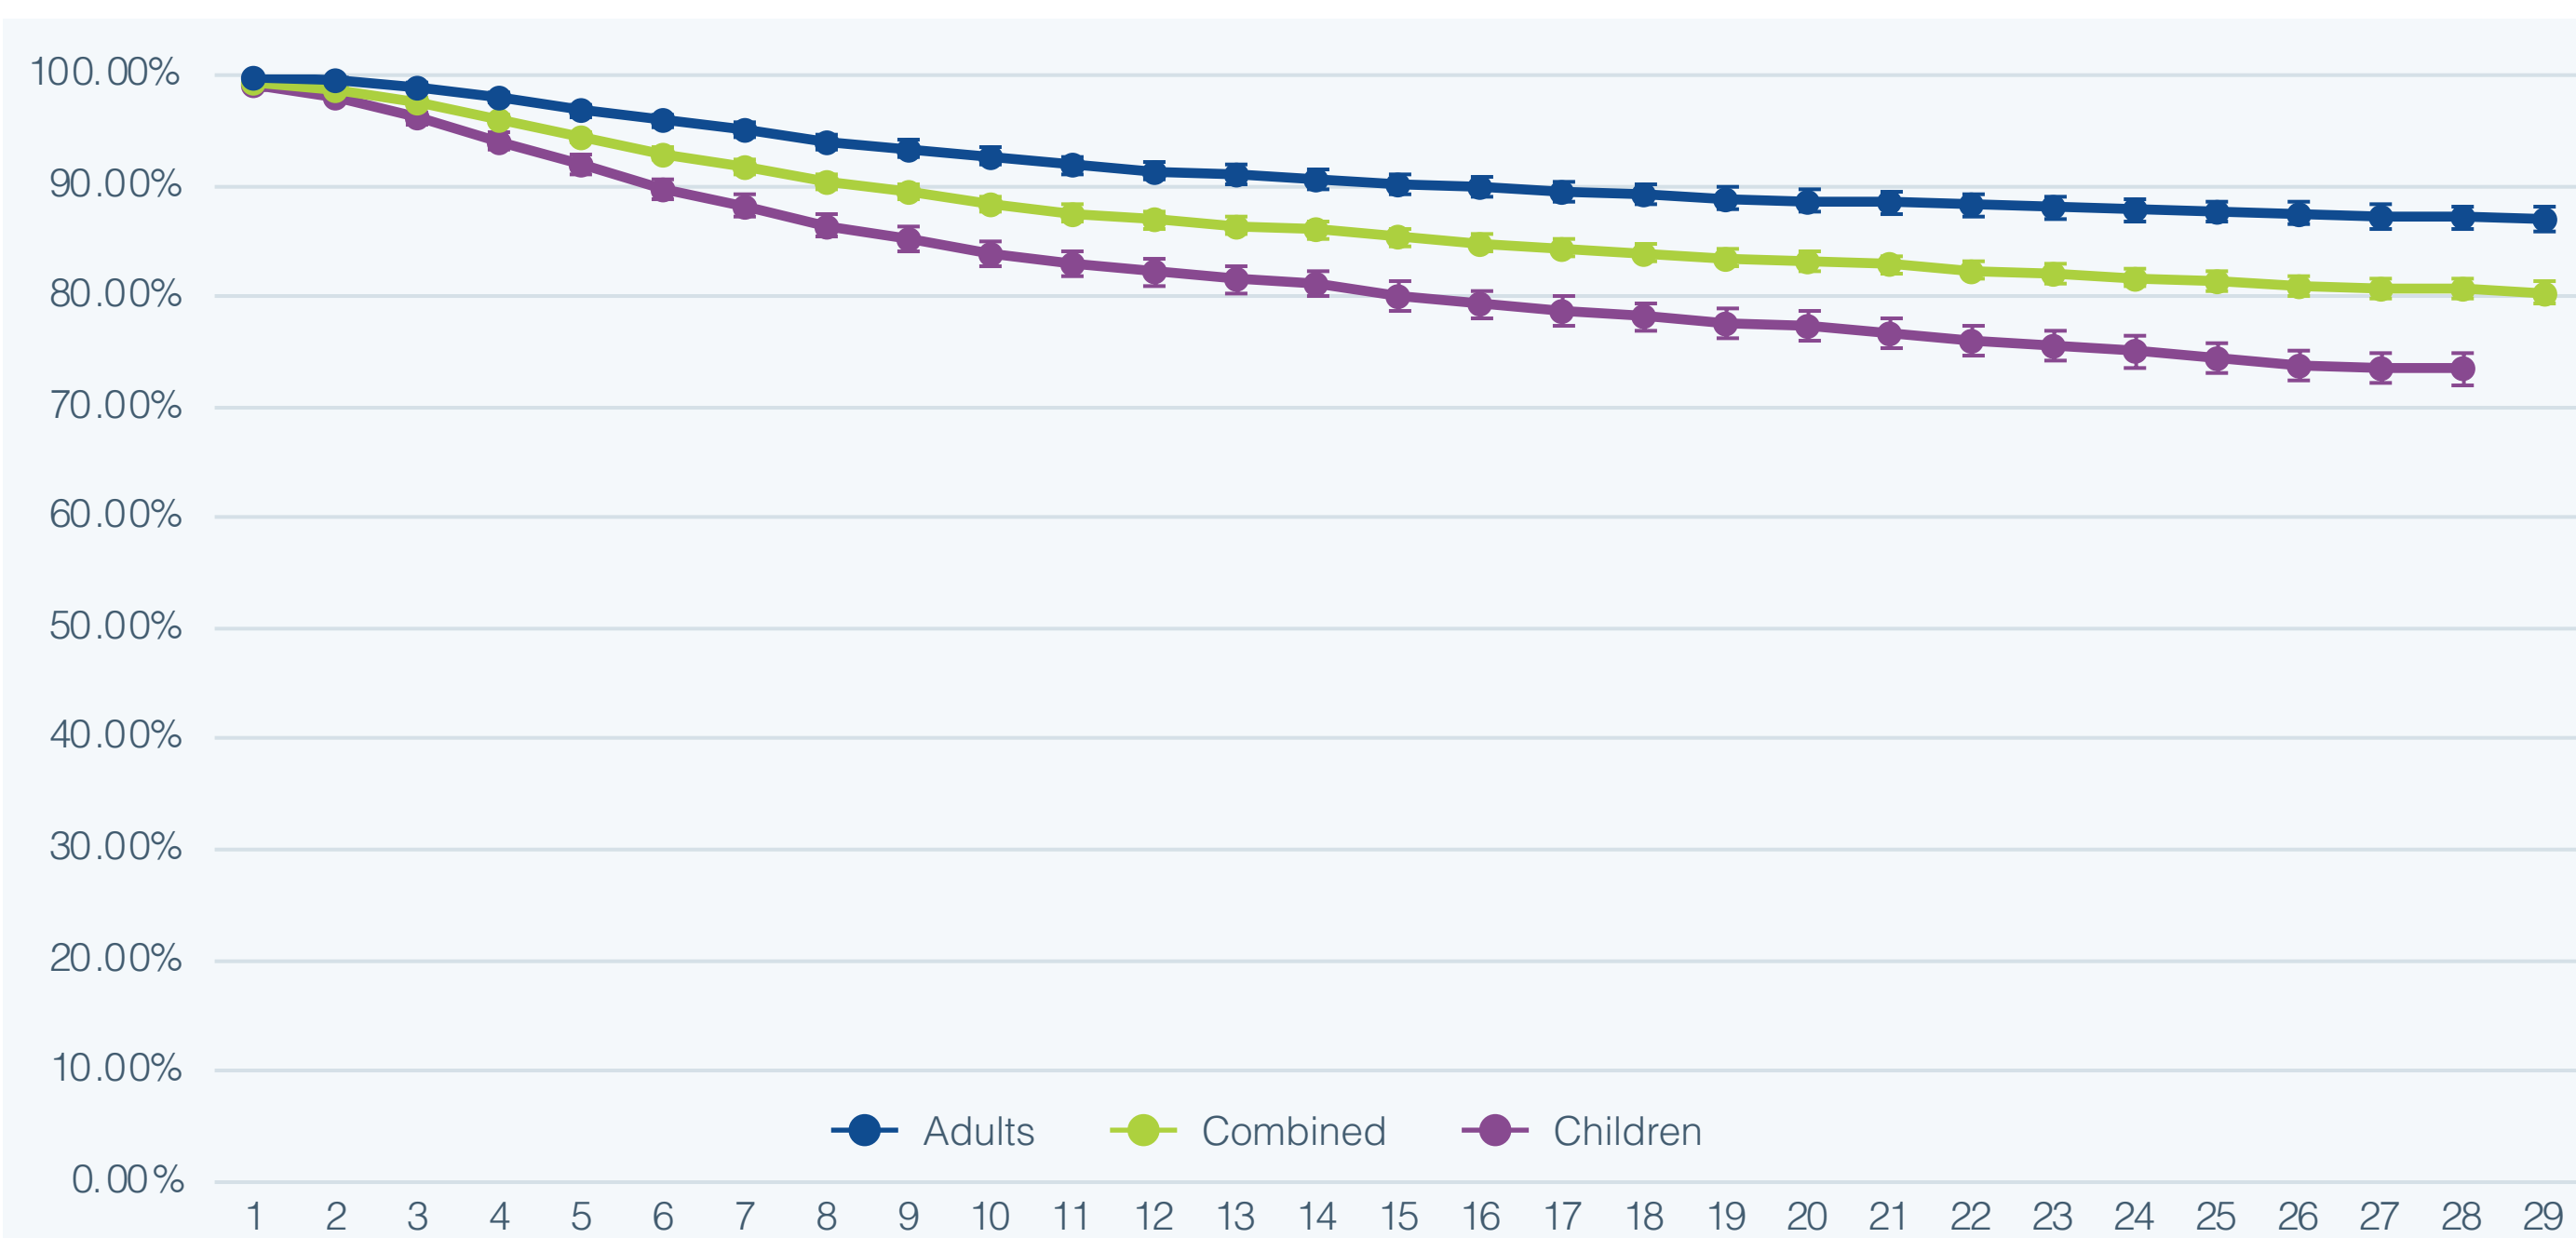

CUMULATIVE SURVIVAL RATE

Years in use	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15
ADULTS	99.84%	99.63%	99.00%	98.02%	96.82%	95.94%	95.06%	94.04%	93.42%	92.67%	91.90%	91.39%	91.02%	90.60%	90.28%
COMBINED	99.47%	98.80%	97.62%	96.11%	94.45%	92.92%	91.77%	90.37%	89.46%	88.40%	87.57%	86.97%	86.47%	86.06%	85.36%
CHILDREN	99.08%	97.93%	96.15%	94.09%	91.94%	89.72%	88.27%	86.46%	85.24%	83.84%	82.94%	82.24%	81.60%	81.19%	80.06%

Years in use	16	17	18	19	20	21	22	23	24	25	26	27	28	29
ADULTS	89.99%	89.57%	89.27%	88.94%	88.66%	88.53%	88.33%	88.07%	87.83%	87.72%	87.55%	87.27%	87.19%	87.06%
COMBINED	84.85%	84.38%	83.94%	83.53%	83.22%	82.89%	82.43%	82.13%	81.73%	81.40%	81.03%	80.79%	80.70%	80.40%
CHILDREN	79.31%	78.78%	78.18%	77.68%	77.33%	76.76%	75.99%	75.64%	75.04%	74.42%	73.76%	73.58%	73.47%	N/A*

*Sample size is not large enough for reporting.

ANSI/AAMI CI86

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

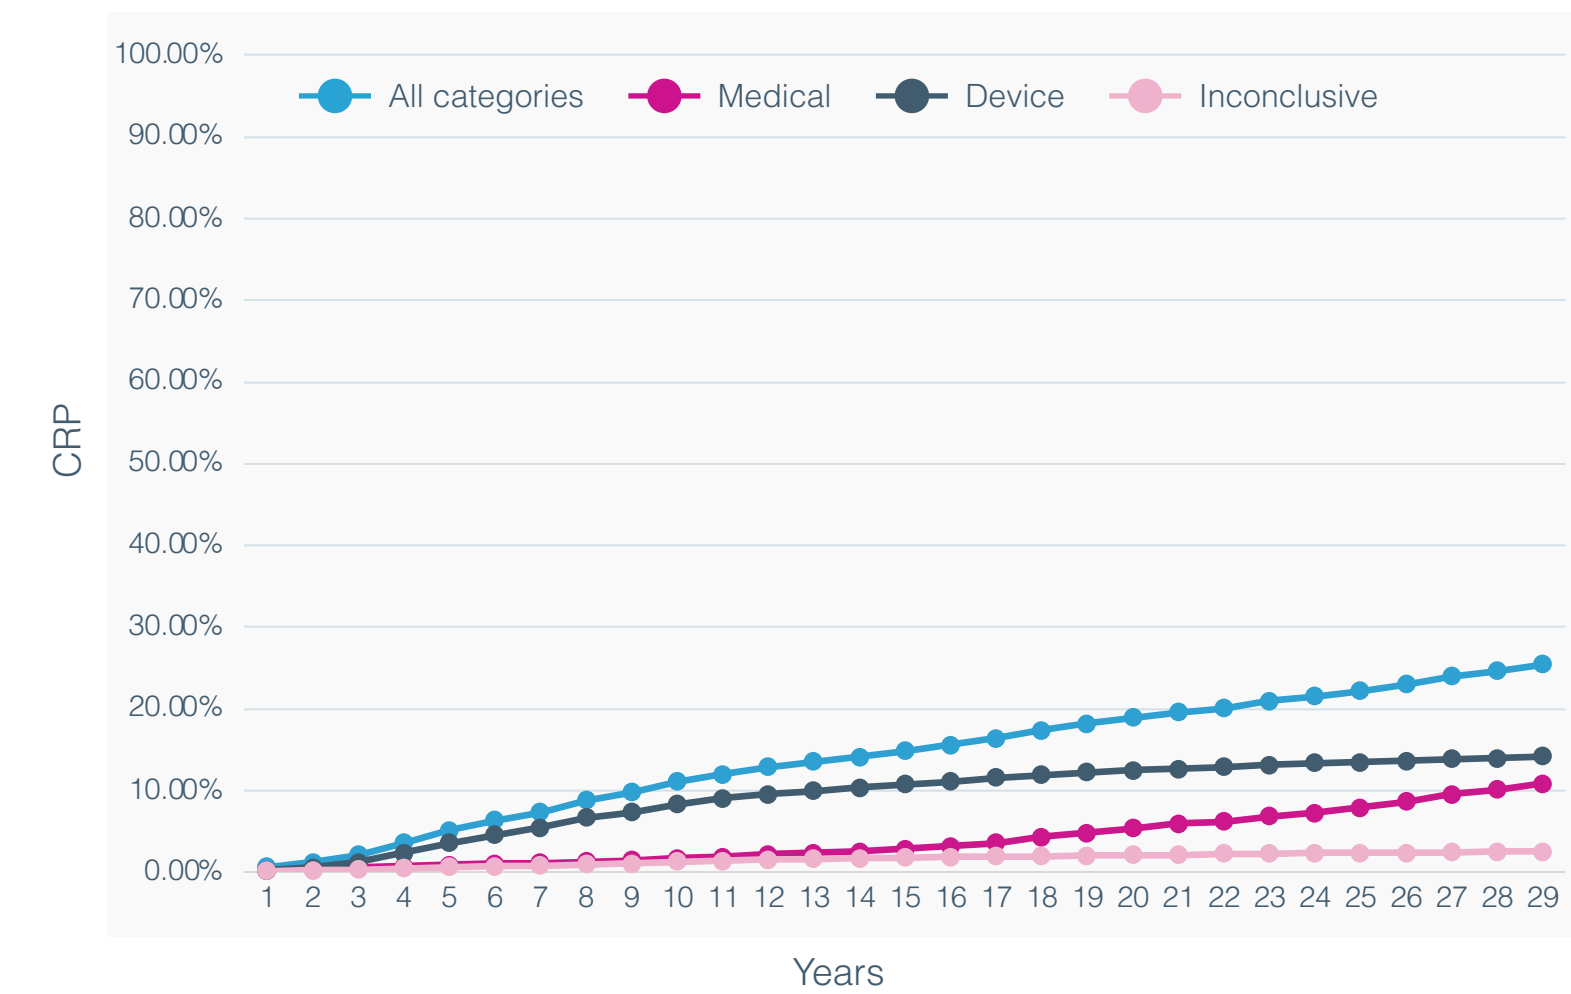

REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

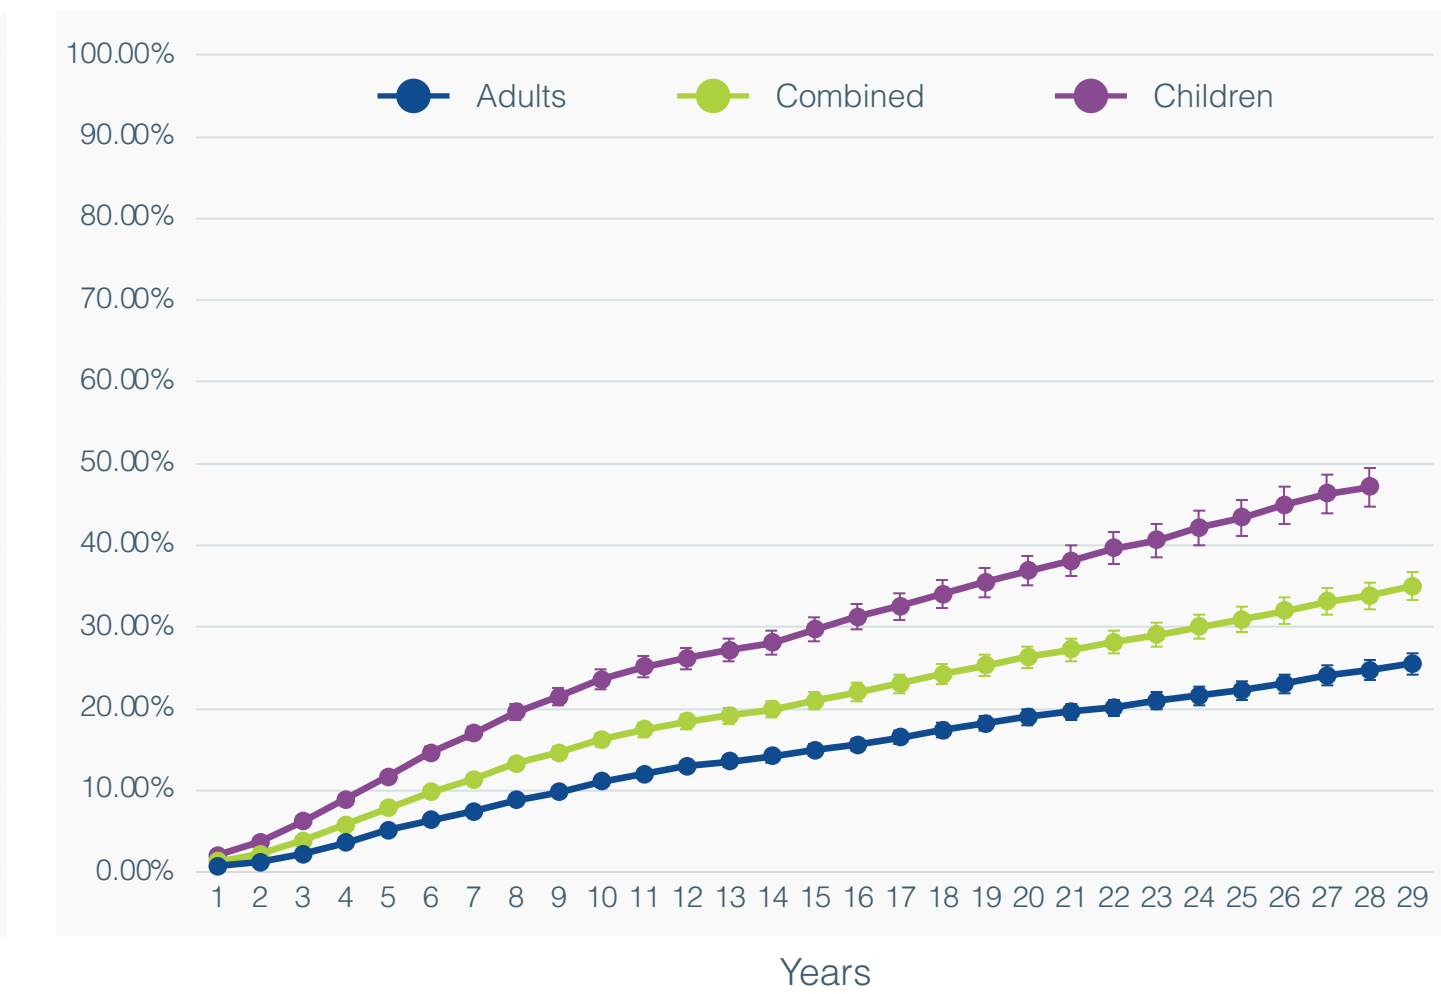

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

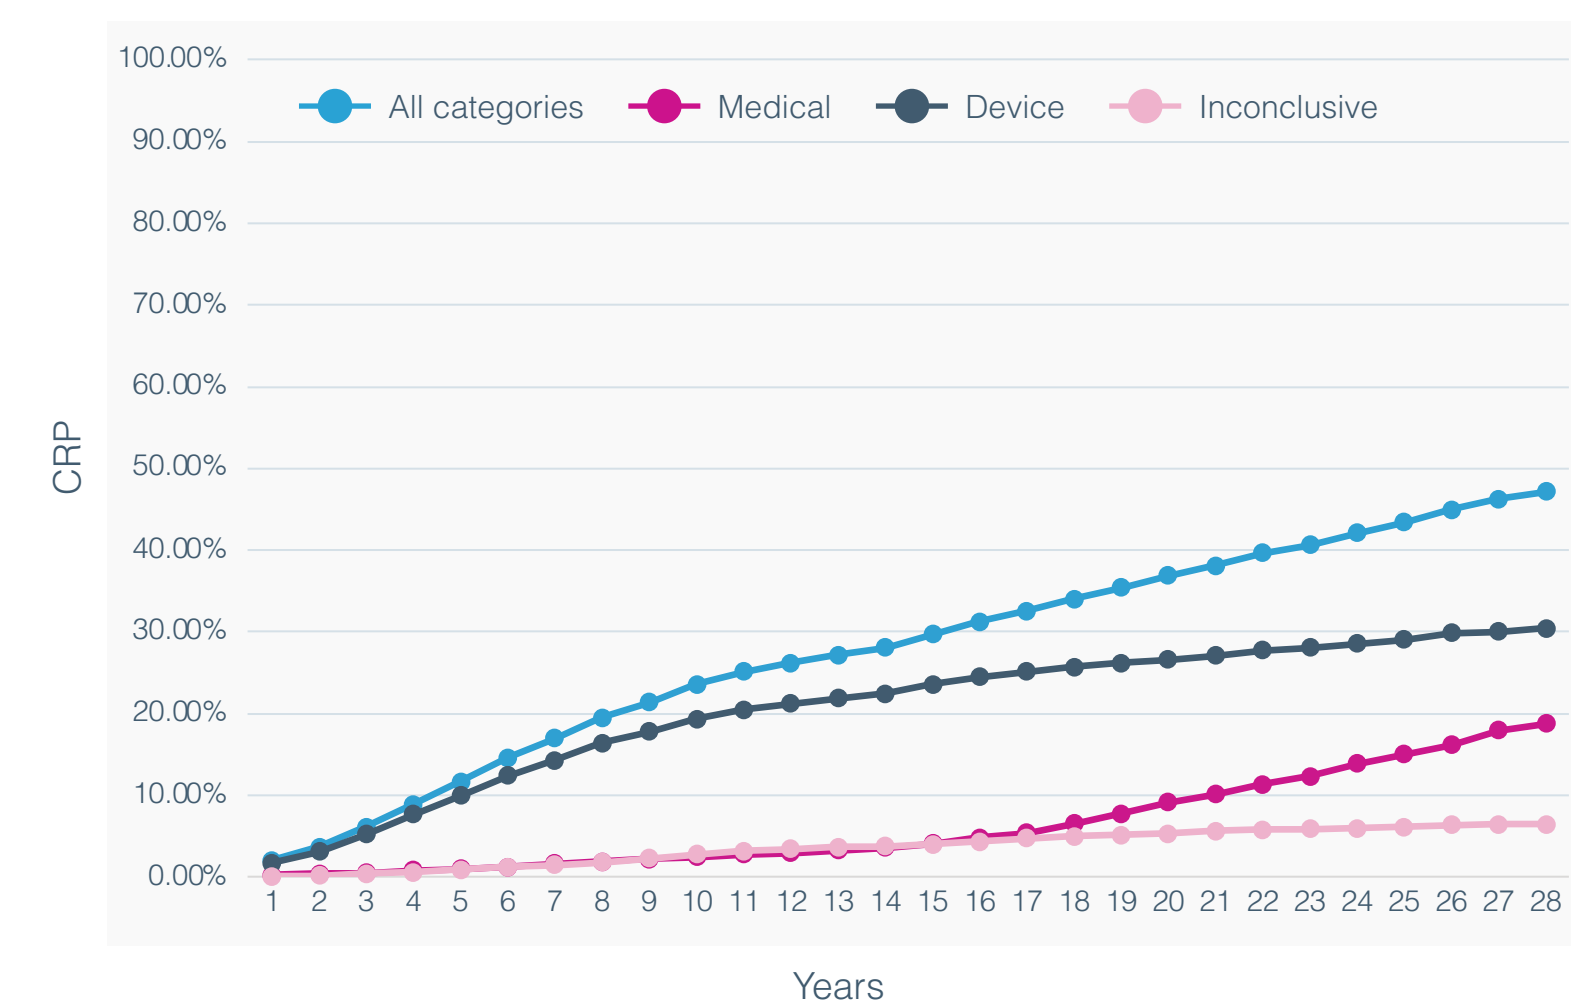

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

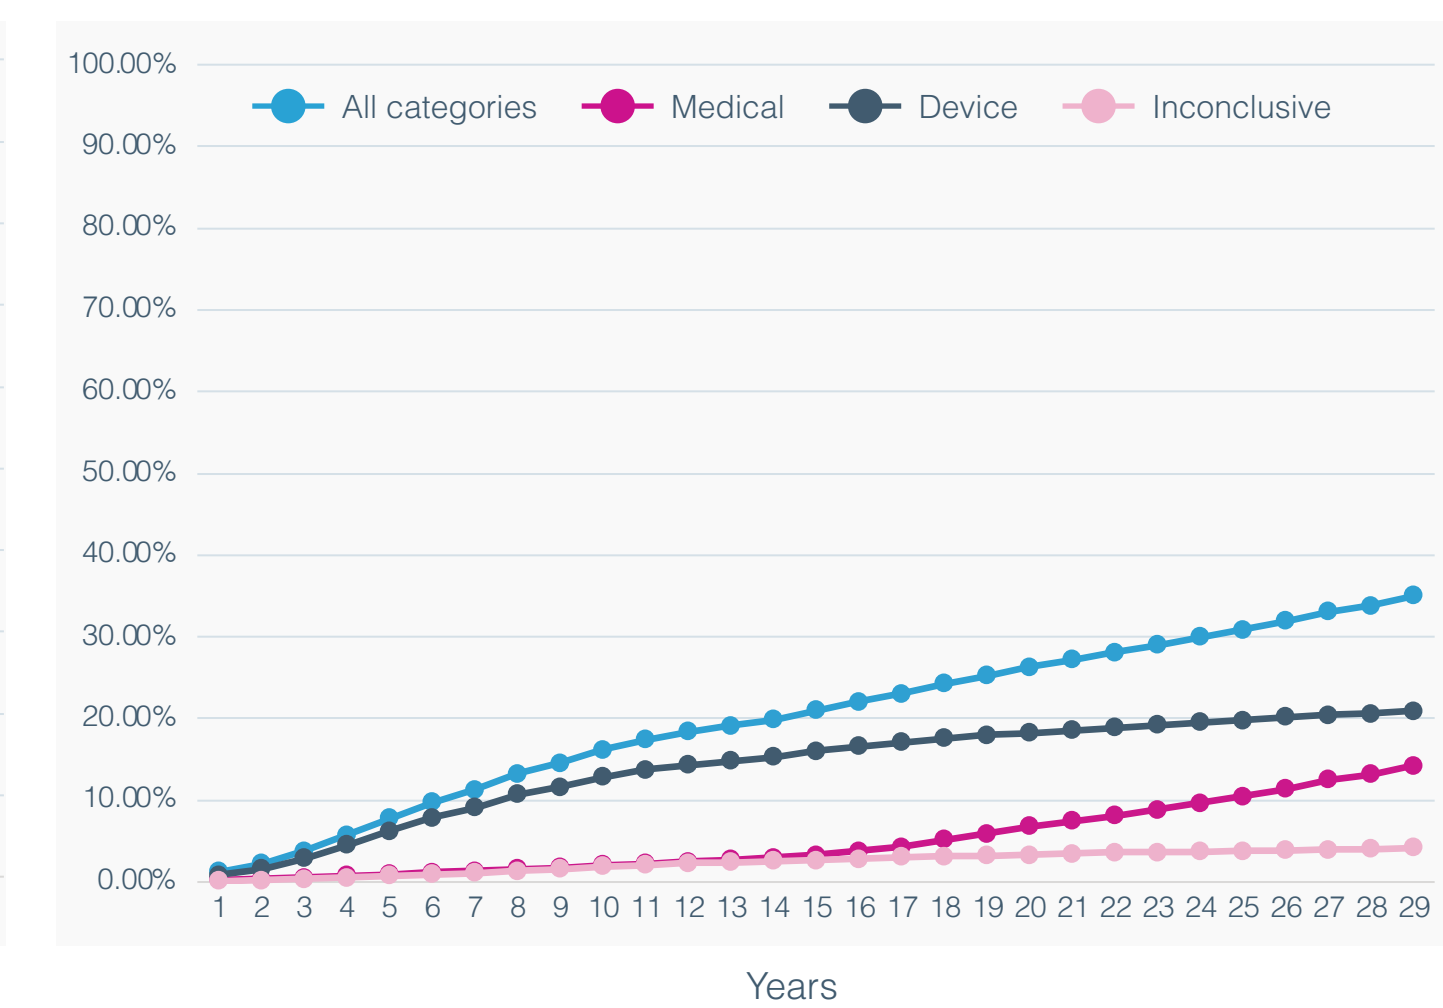

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	Total CI Lower
1	0.26%	0.86%	0.13%	1.25%	1.48%	1.01%
2	0.38%	1.62%	0.23%	2.22%	2.53%	1.90%
3	0.55%	2.91%	0.37%	3.80%	4.21%	3.39%
4	0.78%	4.53%	0.52%	5.77%	6.27%	5.27%
5	0.94%	6.23%	0.76%	7.81%	8.38%	7.24%
6	1.16%	7.84%	0.93%	9.75%	10.38%	9.12%
7	1.34%	9.13%	1.09%	11.32%	12.00%	10.64%
8	1.57%	10.69%	1.30%	13.24%	13.96%	12.51%
9	1.79%	11.65%	1.55%	14.57%	15.33%	13.82%
10	2.03%	12.84%	1.88%	16.22%	17.01%	15.44%
11	2.23%	13.73%	2.08%	17.41%	18.22%	16.60%
12	2.50%	14.31%	2.31%	18.38%	19.21%	17.55%
13	2.72%	14.84%	2.42%	19.16%	20.00%	18.32%
14	2.95%	15.32%	2.52%	19.89%	20.74%	19.04%
15	3.32%	16.03%	2.66%	20.97%	21.84%	20.10%
16	3.82%	16.58%	2.82%	22.03%	22.92%	21.14%
17	4.30%	17.10%	3.02%	23.05%	23.96%	22.15%
18	5.16%	17.56%	3.09%	24.23%	25.14%	23.31%
19	5.90%	17.95%	3.22%	25.28%	26.21%	24.35%
20	6.79%	18.24%	3.33%	26.32%	27.27%	25.38%
21	7.45%	18.52%	3.46%	27.20%	28.15%	26.24%
22	8.07%	18.92%	3.59%	28.14%	29.10%	27.17%
23	8.85%	19.20%	3.62%	29.01%	29.99%	28.04%
24	9.66%	19.52%	3.71%	29.99%	30.97%	29.01%
25	10.46%	19.79%	3.76%	30.88%	31.88%	29.89%
26	11.35%	20.18%	3.85%	31.97%	32.98%	30.95%
27	12.49%	20.42%	3.95%	33.10%	34.15%	32.06%
28	13.18%	20.58%	4.00%	33.81%	34.89%	32.73%
29	14.26%	20.89%	4.18%	35.00%	36.19%	33.82%

Please see the **Appendix** for a complete data set.

CLARION 1.0

The Clarion 1.0 (C1.0) implant was Advanced Bionics first device, the start of a technology-forward lineage that continues today. As the number of children implanted with the C1.0 is below the level required for statistical analysis, the data is included in the combined data.

NUMBER OF REGISTERED C1.0 IMPLANTS

As of April 1, 2026.
Last year of distribution: 1997.[a]

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	294	50	344[b]
ANSI/AAMI CI86	–	–	–

a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.

ISO 5841-2:2014

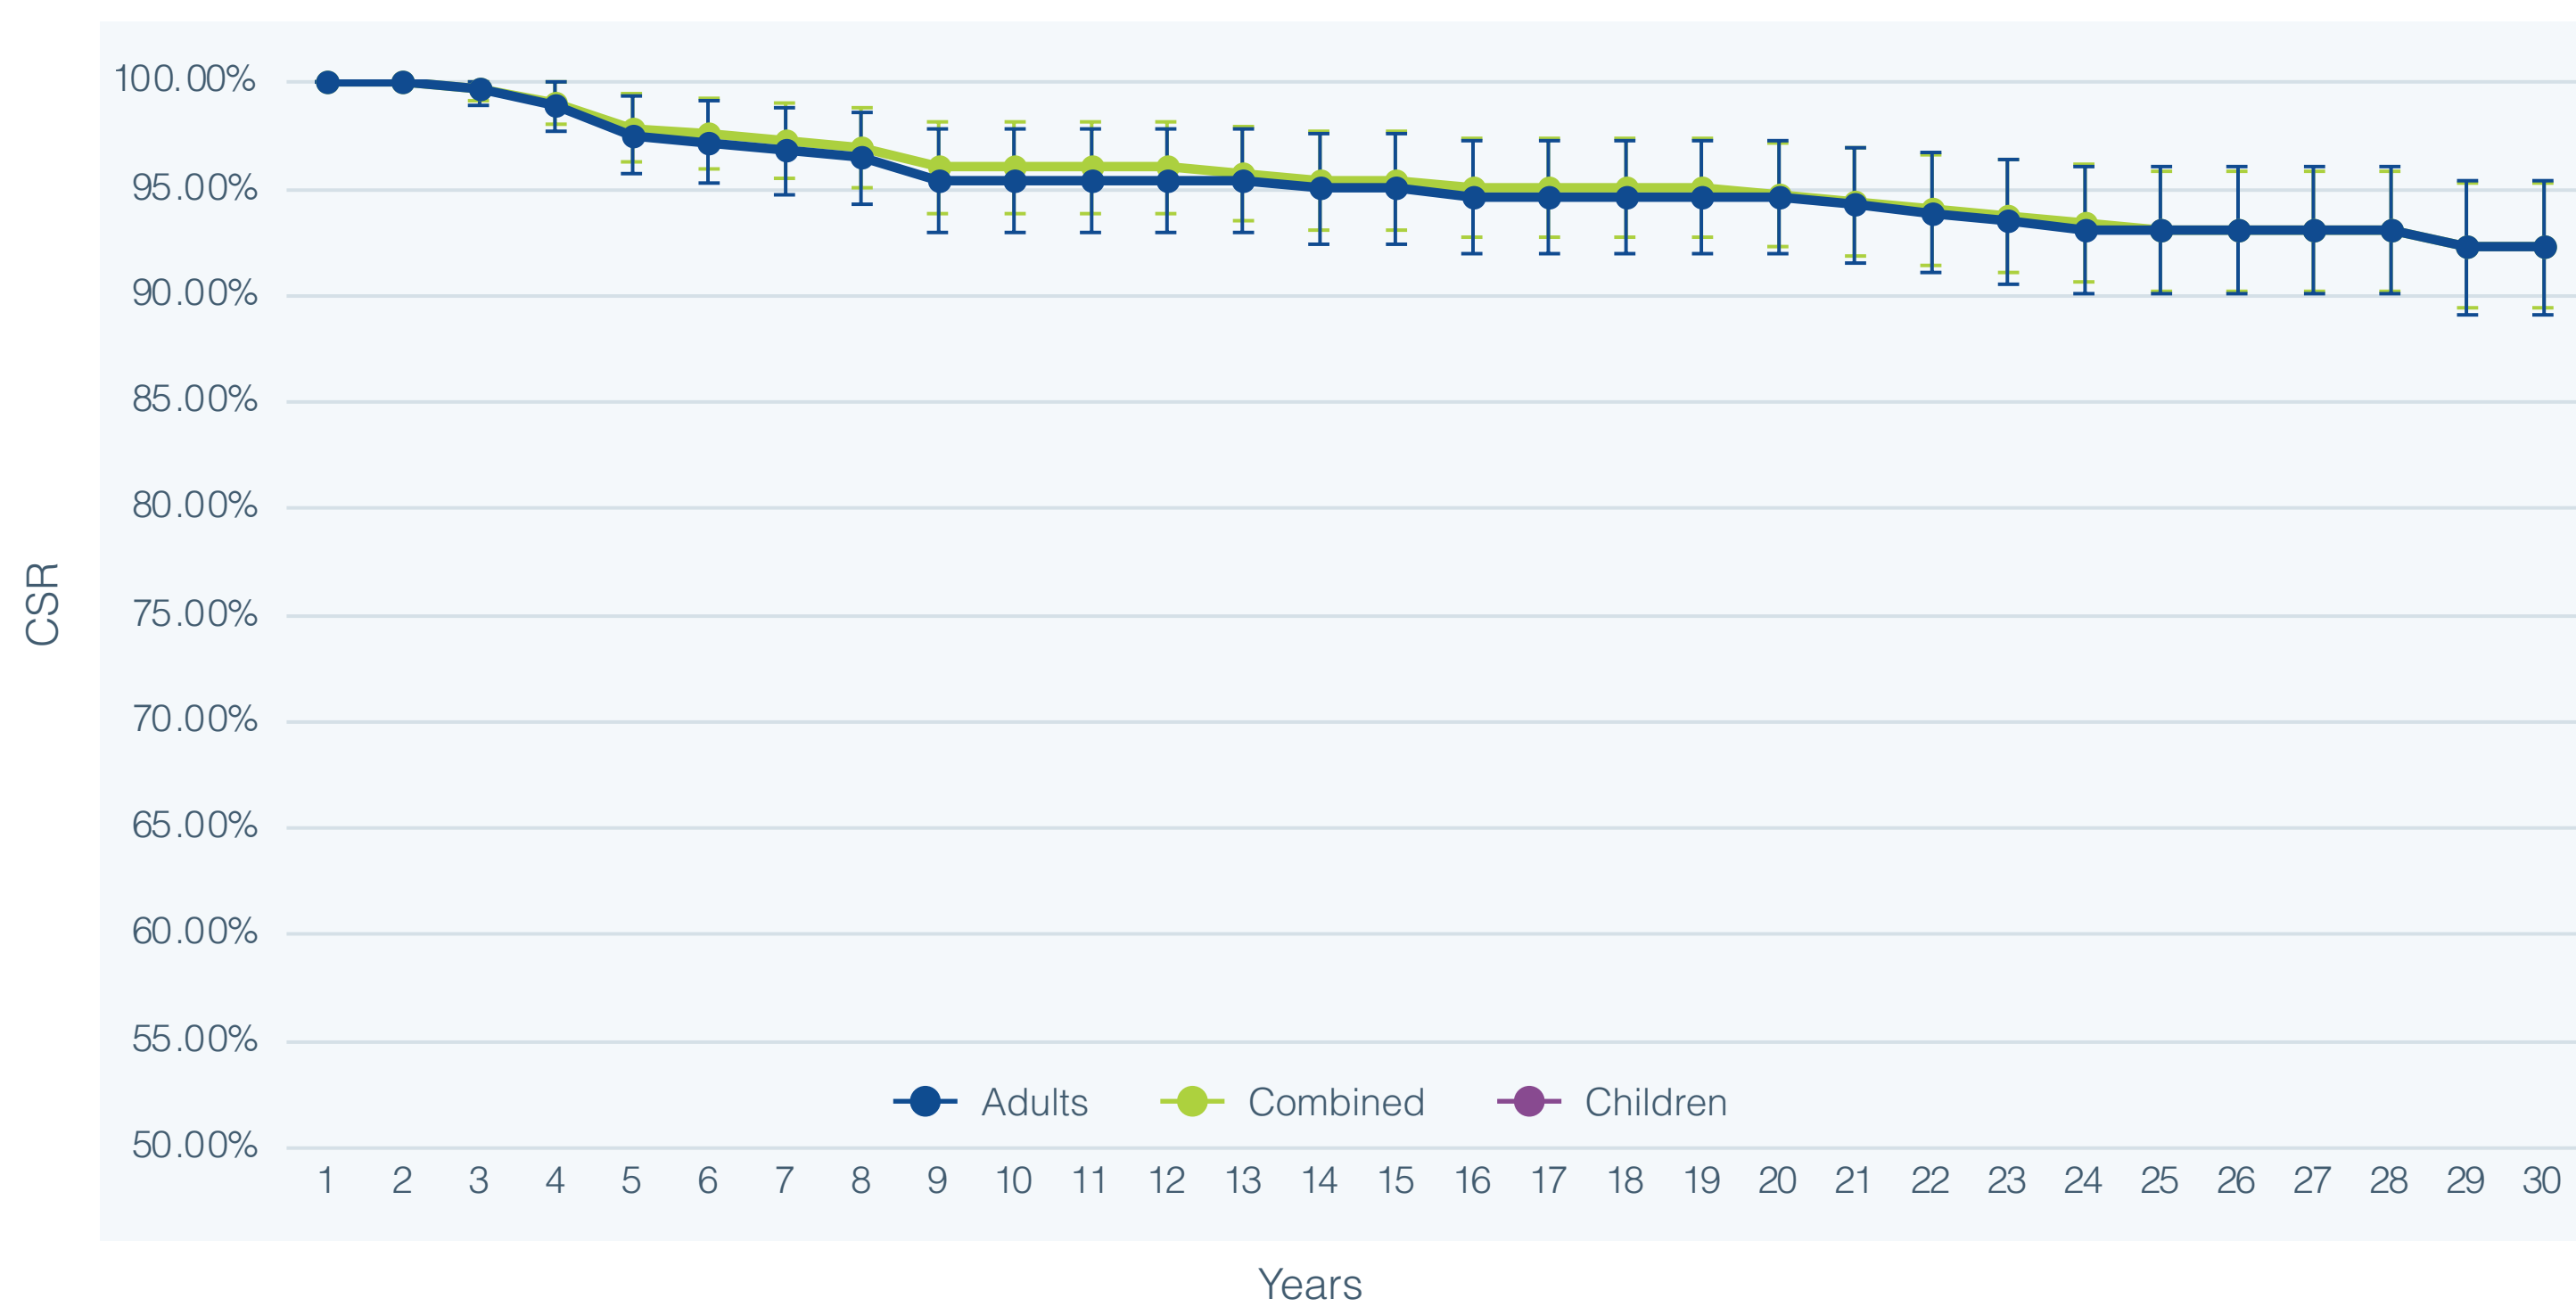

CUMULATIVE SURVIVAL RATE

Years in use	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15
ADULTS	100.00%	100.00%	99.65%	98.94%	97.52%	97.16%	96.81%	96.45%	95.37%	95.37%	95.37%	95.37%	95.37%	95.00%	95.00%
COMBINED	100.00%	100.00%	99.70%	99.09%	97.87%	97.56%	97.25%	96.94%	96.02%	96.02%	96.02%	96.02%	95.70%	95.38%	95.38%

Years in use	16	17	18	19	20	21	22	23	24	25	26	27	28	29	30
ADULTS	94.63%	94.63%	94.63%	94.63%	94.63%	94.24%	93.86%	93.47%	93.08%	93.08%	93.08%	93.08%	93.08%	92.25%	92.25%
COMBINED	95.05%	95.05%	95.05%	95.05%	94.72%	94.39%	94.06%	93.72%	93.38%	93.04%	93.04%	93.04%	93.04%	92.33%	92.33%

ANSI/AAMI CI86

The ANSI/AAMI CI86 Standard does not require reporting for devices older than 20 years after the last implantation of that device type. Please refer to the ISO data for information.

Please see the **Appendix** for a complete data set.

For each currently-available sound processor, there will be a simple measure of reliability based on the average global yearly return rate and graphical data in compliance with ANSI/AAMI CI86 Standard that shows the monthly failure rate.

Where possible, this monthly data is further categorized into failure mechanisms, if known, to include mechanical, electronic, moisture damage, and other. Processors that meet all specifications are included and they are classified as no fault found. Where available, the number of registered users is shown, categorized into adult, children, and combined.

NAÍDA CI AND SKY CI MARVEL

The Naída™ CI M sound processor for adults and Sky CI™ M sound processor for children are the newest Advanced Bionics products integrated with the latest advancements from Phonak, the Marvel platform. With built-in connectivity solutions and the ability to automatically sense and adapt to every situation, the Naída CI M and Sky CI M processors are designed to give you the best hearing experience.

RELIABILITY: 99.61%[a]

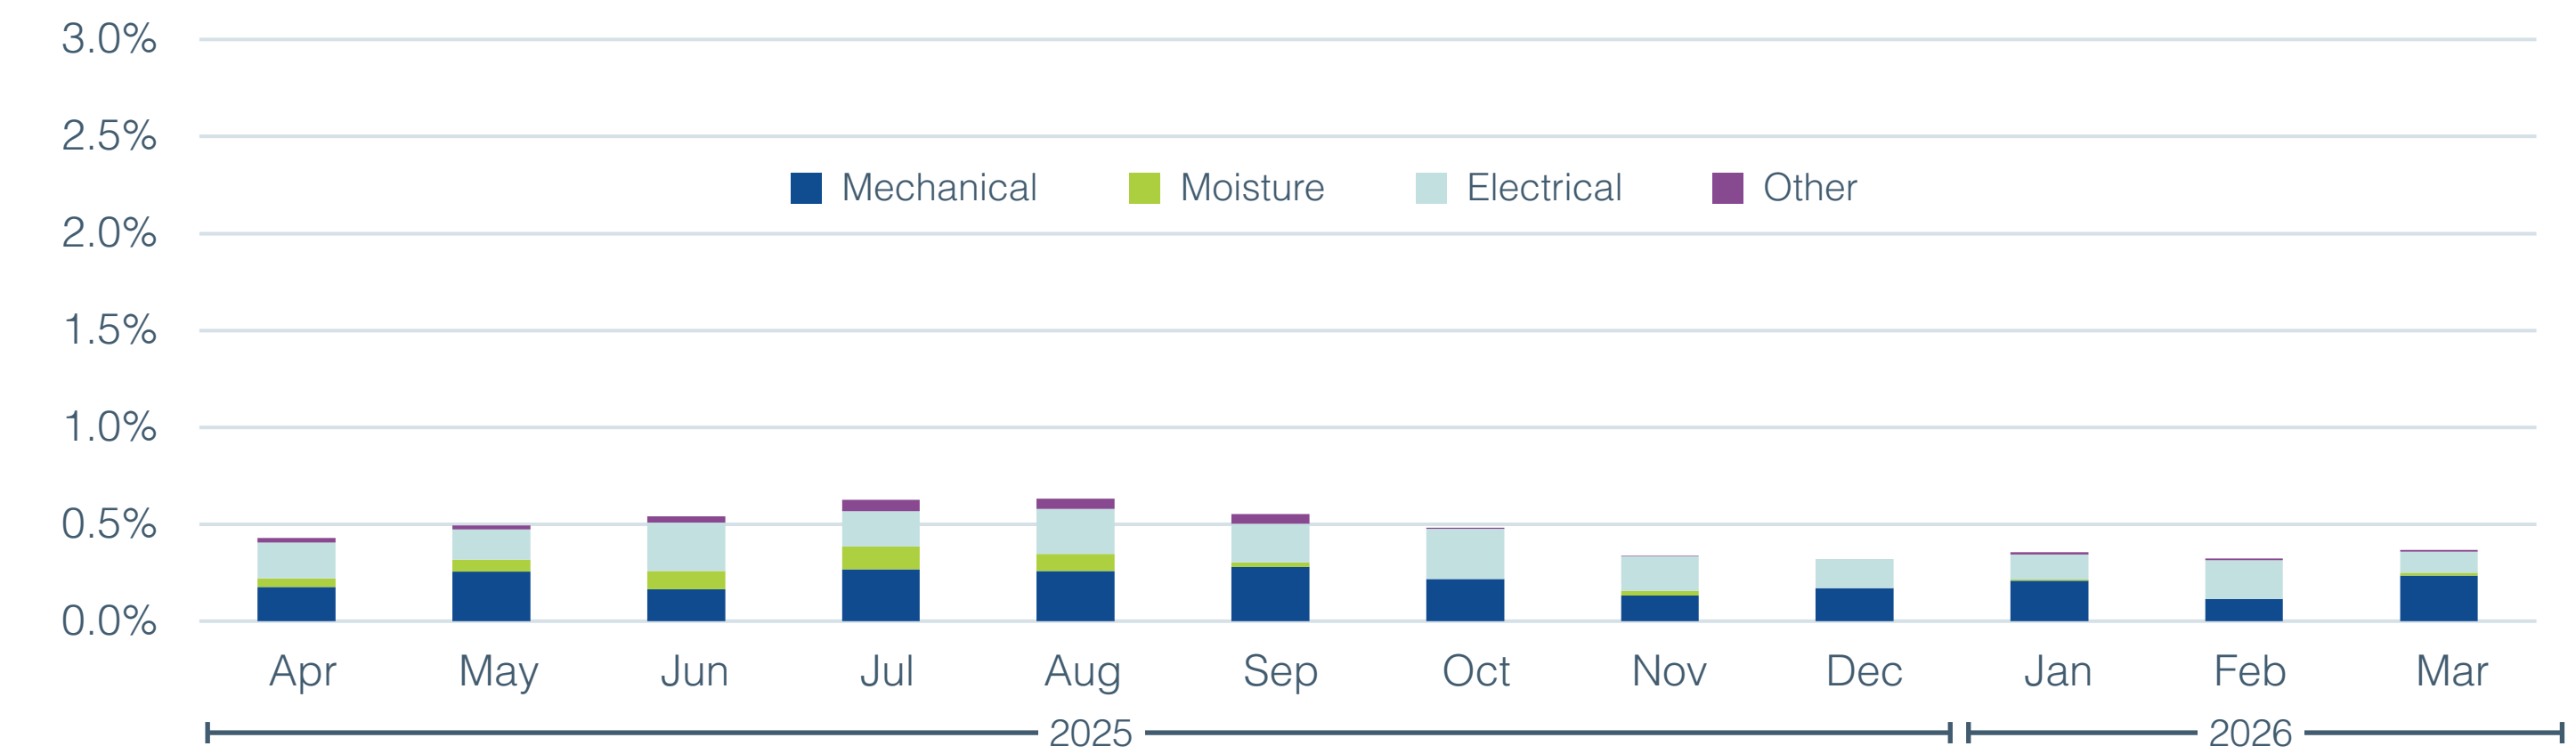

FAILED COMPONENT RETURN RATE[b]

CAUSE	APR 25	MAY 25	JUN 25	JUL 25	AUG 25	SEP 25	OCT 25	NOV 25	DEC 25	JUN 26	FEB 26	MAR 26
MECHANICAL	0.18%	0.26%	0.17%	0.27%	0.26%	0.28%	0.22%	0.13%	0.17%	0.21%	0.12%	0.24%
MOISTURE	0.05%	0.06%	0.09%	0.12%	0.09%	0.02%	0.00%	0.02%	0.00%	0.01%	0.00%	0.01%
ELECTRICAL	0.18%	0.16%	0.25%	0.18%	0.23%	0.20%	0.26%	0.18%	0.15%	0.13%	0.20%	0.11%
OTHER	0.02%	0.02%	0.03%	0.06%	0.05%	0.05%	0.01%	0.00%	0.00%	0.01%	0.01%	0.01%

a. Reliability is 1 minus the return rate. The return rate is the average global monthly return rate between April 2025 and March 2026.
b. The number per month represent the unit that complete failure analysis in that month.

MARVEL CI | ADVANCED BIONICS POWERFUL CONNECTIONS

NAÍDA CI Q SERIES

The Naída™ CI Q sound processors feature state-of-the-art technologies exclusively available from Advanced Bionics and Phonak for the best possible hearing experience.

RELIABILITY: 99.99%[a]

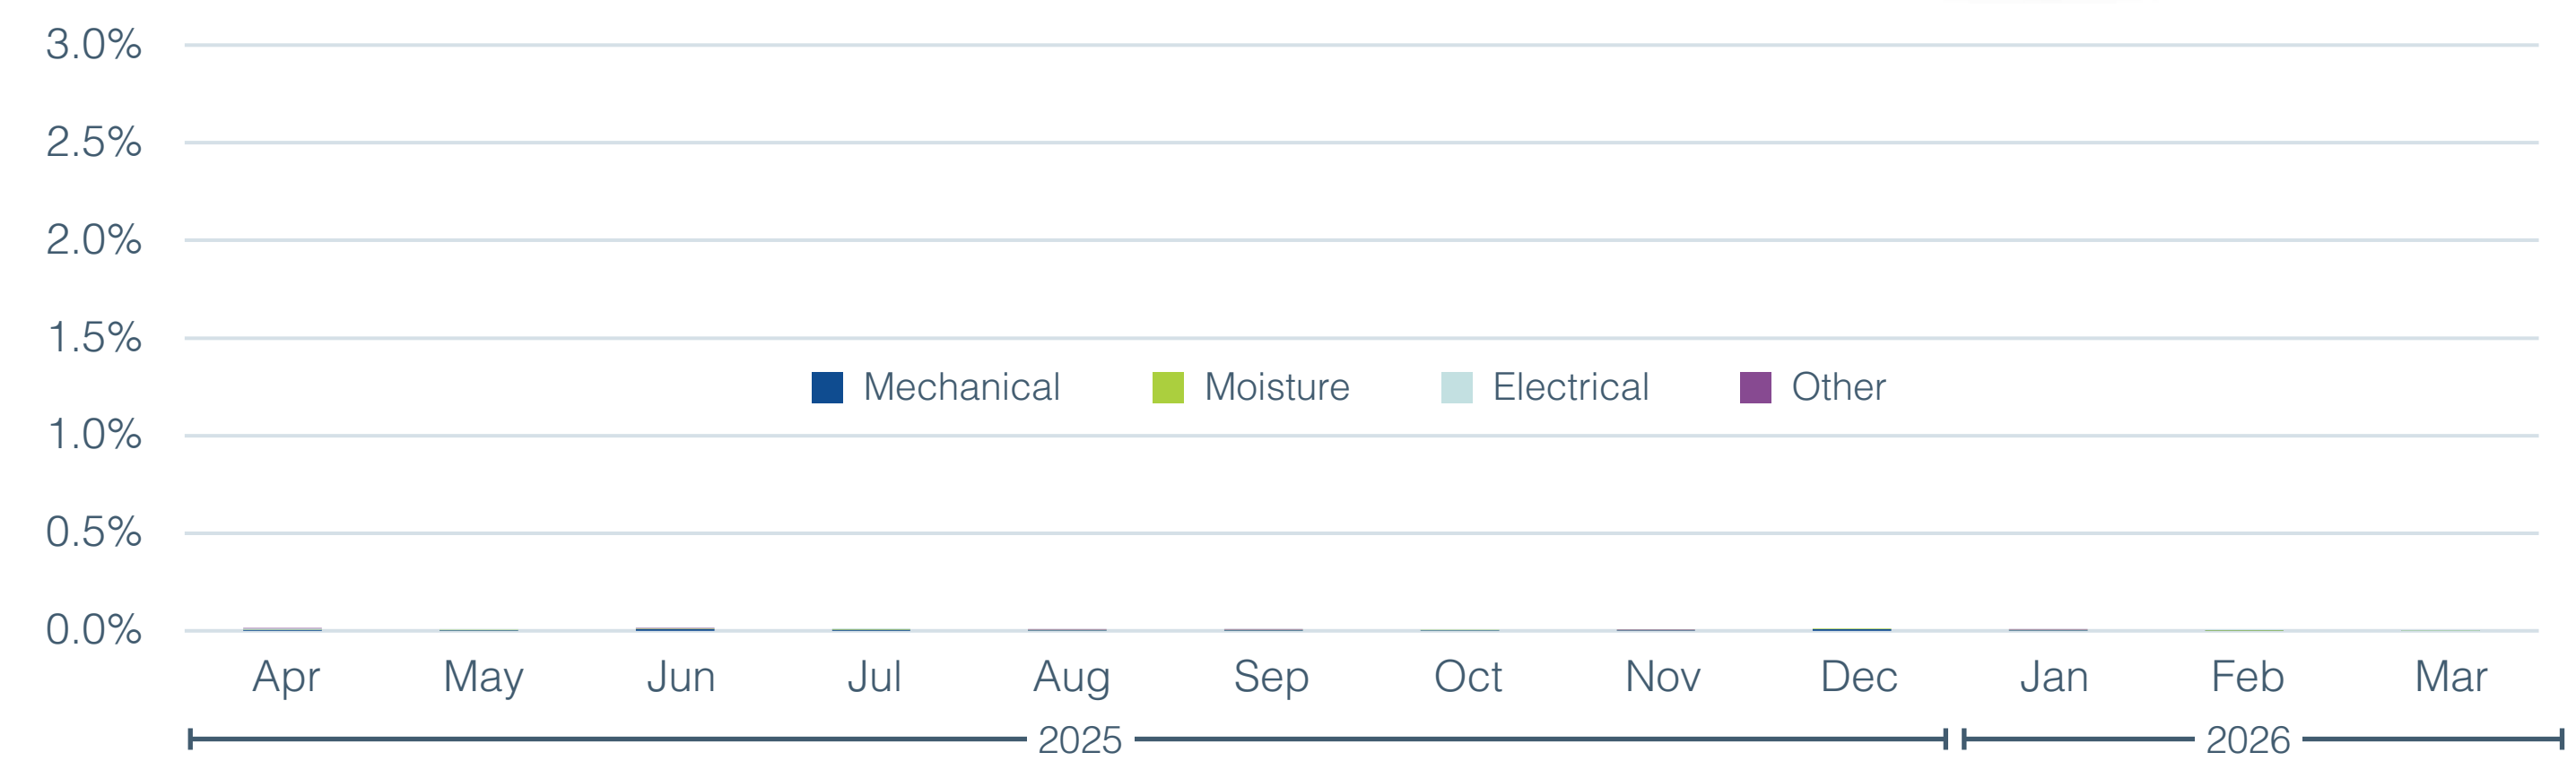

FAILED COMPONENT RETURN RATE[b]

CAUSE	APR 25	MAY 25	JUN 25	JUL 25	AUG 25	SEP 25	OCT 25	NOV 25	DEC 25	JUN 26	FEB 26	MAR 26
MECHANICAL	0.01%	0.00%	0.01%	0.01%	0.00%	0.00%	0.00%	0.00%	0.01%	0.00%	0.00%	0.00%
MOISTURE	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%
ELECTRICAL	0.01%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%
OTHER	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%

CHORUS

The Chorus™ sound processor is compatible with C1.0 and C1.2 cochlear implants, and offers integrated Roger™ technology for connectivity and performance.

RELIABILITY: 99.87%[a]

Number of returned products is too low to report on failed component return rates.

a. Reliability is 1 minus the return rate. The return rate is the average global monthly return rate between April 2025 and March 2026.
b. The number per month represent the unit that complete failure analysis in that month.

NEPTUNE

The Neptune™ sound processor is the first and only swimmable sound processor.

RELIABILITY: 100%[a]

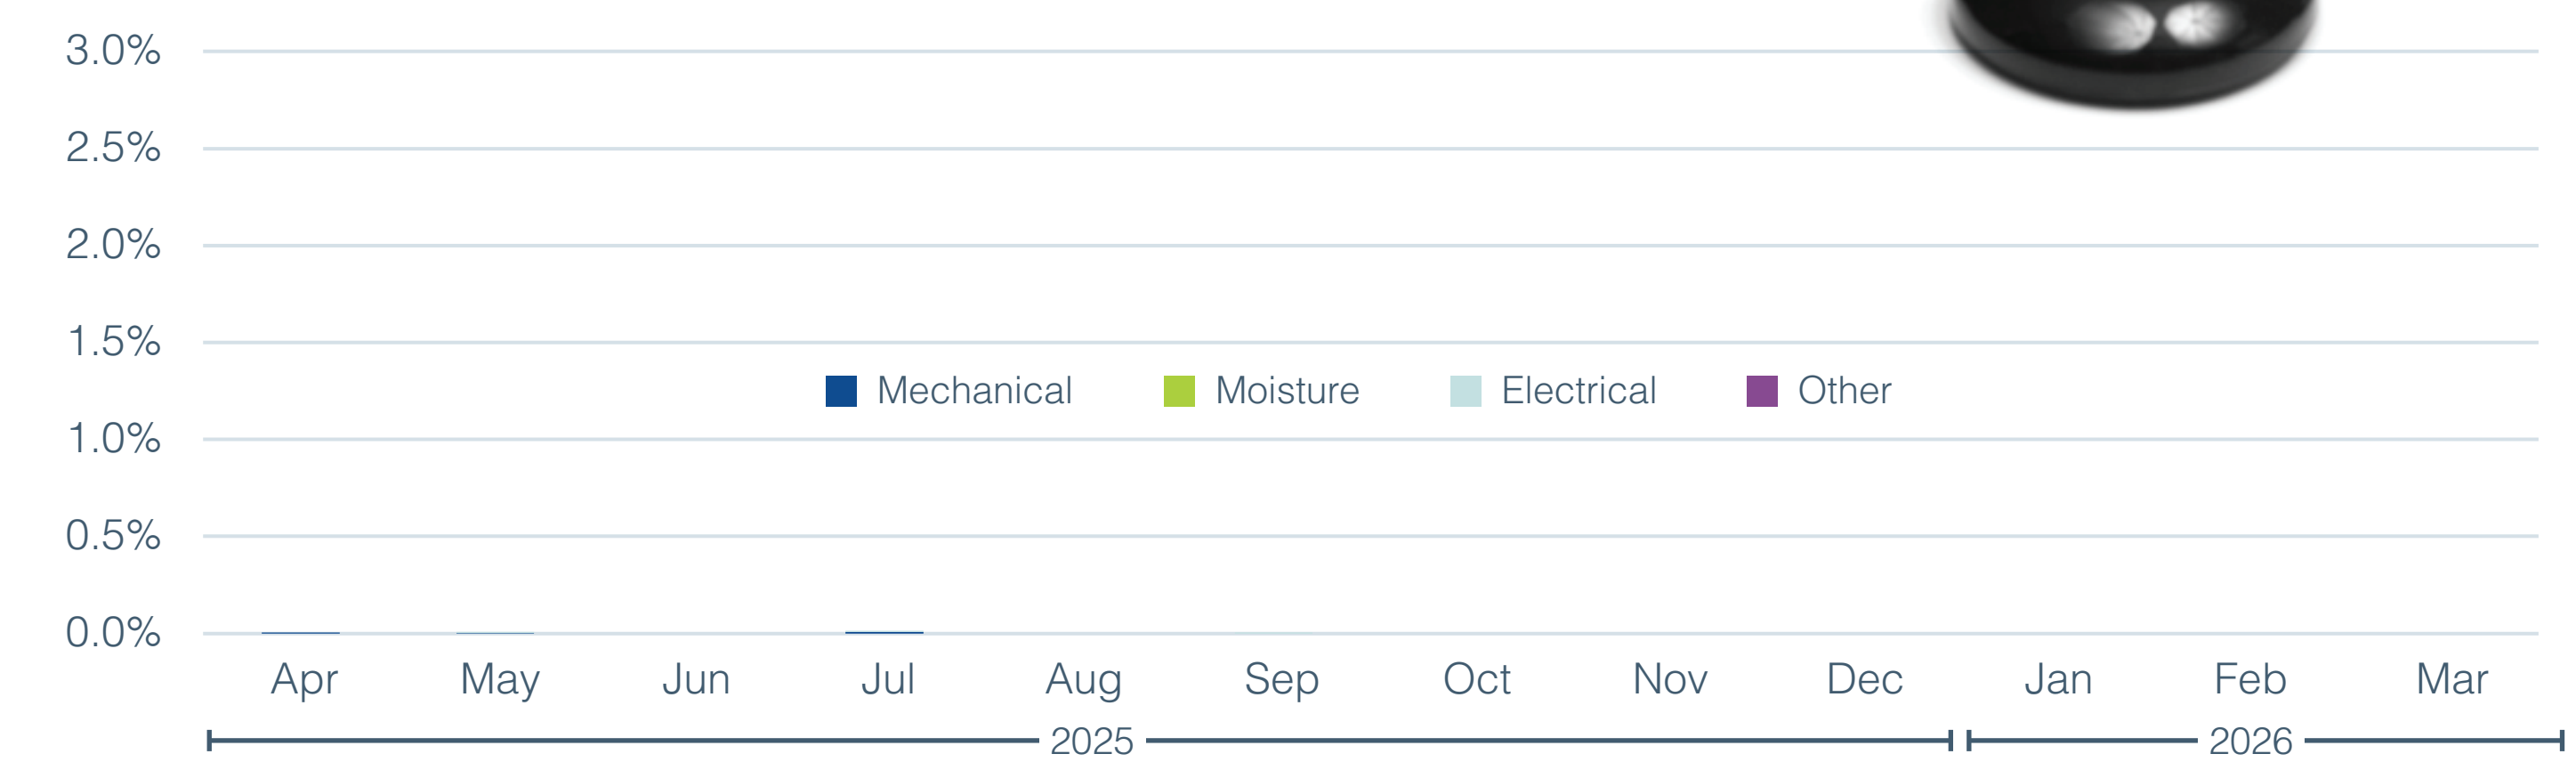

FAILED COMPONENT RETURN RATE[b]

CAUSE	APR 25	MAY 25	JUN 25	JUL 25	AUG 25	SEP 25	OCT 25	NOV 25	DEC 25	JUN 26	FEB 26	MAR 26
MECHANICAL	0.00%	0.00%	0.00%	0.01%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%
MOISTURE	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%
ELECTRICAL	0.00%	0.01%	0.00%	0.01%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%
OTHER	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%

a. Reliability is 1 minus the return rate. The return rate is the average global monthly return rate between April 2025 and March 2026.
b. The number per month represent the unit that complete failure analysis in that month.

HIRES ULTRA 3D V2

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
						CI Higher	CI Lower
	1	0.76%	0.02%	0.01%	0.79%	0.88%	0.70%
	1.5	0.98%	0.03%	0.01%	1.02%	1.12%	0.91%
	2	1.19%	0.04%	0.01%	1.24%	1.36%	1.12%
	2.5	1.36%	0.04%	0.01%	1.42%	1.55%	1.29%
	3	1.49%	0.05%	0.02%	1.56%	1.70%	1.41%
ADULTS	3.5	1.64%	0.05%	0.02%	1.71%	1.86%	1.55%
	4	1.76%	0.05%	0.02%	1.83%	2.00%	1.66%
	4.5	1.81%	0.06%	0.02%	1.89%	2.07%	1.71%
	5	1.90%	0.06%	0.02%	1.98%	2.17%	1.78%
	5.5	1.93%	0.06%	0.02%	2.00%	2.20%	1.80%
	6	1.93%	0.06%	0.02%	2.00%	2.20%	1.80%
	1	0.56%	0.05%	0.01%	0.62%	0.78%	0.46%
	1.5	0.68%	0.09%	0.01%	0.78%	0.97%	0.60%
	2	0.78%	0.11%	0.01%	0.89%	1.09%	0.69%
	2.5	0.88%	0.20%	0.01%	1.08%	1.32%	0.85%
	3	0.88%	0.22%	0.01%	1.11%	1.34%	0.87%
CHILDREN	3.5	1.03%	0.27%	0.04%	1.33%	1.61%	1.06%
	4	1.21%	0.27%	0.04%	1.51%	1.82%	1.20%
	4.5	1.26%	0.27%	0.04%	1.56%	1.88%	1.23%
	5	1.43%	0.33%	0.04%	1.79%	2.19%	1.39%
	5.5	1.51%	0.42%	0.04%	1.96%	2.43%	1.50%
	6*	N/A	N/A	N/A	N/A	N/A	N/A

HIRES ULTRA V2

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
						CI Higher	CI Lower
	1	0.42%	0.00%	0.03%	0.45%	0.60%	0.29%
	1.5	0.54%	0.00%	0.04%	0.58%	0.76%	0.40%
	2	0.59%	0.00%	0.04%	0.64%	0.83%	0.45%
	2.5	0.62%	0.00%	0.04%	0.66%	0.85%	0.46%
ADULTS	3	0.67%	0.00%	0.04%	0.71%	0.92%	0.50%
	3.5	0.81%	0.00%	0.08%	0.89%	1.15%	0.63%
	4	0.95%	0.00%	0.08%	1.04%	1.34%	0.73%
	4.5	0.95%	0.00%	0.08%	1.04%	1.34%	0.73%
	5	0.95%	0.00%	0.08%	1.04%	1.34%	0.73%
	5.5*	0.95%	0.00%	0.08%	1.04%	1.34%	0.73%
	1	0.40%	0.06%	0.00%	0.45%	0.59%	0.31%
	1.5	0.42%	0.07%	0.00%	0.49%	0.64%	0.35%
	2	0.44%	0.09%	0.00%	0.52%	0.67%	0.37%
	2.5	0.44%	0.09%	0.00%	0.52%	0.67%	0.37%
CHILDREN	3	0.47%	0.13%	0.00%	0.60%	0.77%	0.43%
	3.5	0.47%	0.13%	0.00%	0.60%	0.77%	0.43%
	4	0.51%	0.13%	0.00%	0.64%	0.83%	0.45%
	4.5	0.51%	0.13%	0.00%	0.64%	0.83%	0.45%
	5	0.51%	0.13%	0.00%	0.64%	0.83%	0.45%
	5.5*	N/A	N/A	N/A	N/A	N/A	N/A

*Sample size is not large enough for reporting.

HIRES ULTRA 3D V1

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
						CI Higher	CI Lower
	1	0.93%	0.15%	0.02%	1.10%	1.39%	0.82%
	1.5	1.41%	0.75%	0.10%	2.25%	2.65%	1.85%
	2	1.76%	2.48%	0.18%	4.37%	4.92%	3.82%
	2.5	2.14%	5.22%	0.22%	7.45%	8.16%	6.74%
	3	2.45%	8.49%	0.24%	10.94%	11.79%	10.10%
	3.5	2.71%	12.70%	0.33%	15.35%	16.32%	14.37%
ADULTS	4	2.91%	16.37%	0.37%	19.11%	20.18%	18.04%
	4.5	3.08%	19.90%	0.37%	22.65%	23.79%	21.52%
	5	3.31%	22.74%	0.40%	25.59%	26.78%	24.40%
	5.5	3.41%	25.67%	0.40%	28.49%	29.73%	27.26%
	6	3.60%	27.95%	0.40%	30.82%	32.08%	29.56%
	6.5	3.63%	29.41%	0.40%	32.24%	33.52%	30.96%
	7	3.63%	30.53%	0.40%	33.32%	34.63%	32.00%
	1	1.10%	0.49%	0.07%	1.65%	2.31%	1.00%
	1.5	1.59%	2.17%	0.07%	3.79%	4.78%	2.81%
	2	2.04%	7.67%	0.22%	9.75%	11.28%	8.22%
	2.5	2.74%	13.27%	0.22%	15.83%	17.71%	13.94%
	3	3.93%	19.75%	0.22%	23.07%	25.26%	20.89%
	3.5	4.11%	25.52%	0.31%	28.81%	31.15%	26.46%
CHILDREN	4	4.61%	32.07%	0.31%	35.41%	37.89%	32.92%
	4.5	5.82%	37.65%	0.31%	41.46%	44.03%	38.90%
	5	6.06%	41.71%	0.31%	45.41%	48.01%	42.82%
	5.5	6.57%	44.95%	0.31%	48.73%	51.34%	46.12%
	6	6.70%	48.01%	0.31%	51.65%	54.26%	49.03%
	6.5	6.85%	50.63%	0.31%	54.16%	56.77%	51.54%
	7*	N/A	N/A	N/A	N/A	N/A	N/A

HIRES ULTRA V2

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
						CI Higher	CI Lower
	1	0.78%	0.02%	0.02%	0.83%	1.02%	0.64%
	1.5	1.04%	0.09%	0.02%	1.16%	1.38%	0.93%
	2	1.31%	0.44%	0.05%	1.79%	2.07%	1.51%
	2.5	1.59%	1.41%	0.08%	3.07%	3.43%	2.70%
	3	1.76%	3.28%	0.11%	5.08%	5.55%	4.62%
	3.5	1.91%	6.06%	0.15%	7.99%	8.57%	7.41%
	4	2.00%	9.27%	0.16%	11.23%	11.90%	10.55%
	4.5	2.08%	12.59%	0.19%	14.57%	15.32%	13.82%
ADULTS	5	2.19%	16.18%	0.20%	18.19%	19.01%	17.36%
	5.5	2.31%	19.54%	0.23%	21.57%	22.45%	20.70%
	6	2.45%	22.07%	0.25%	24.16%	25.07%	23.24%
	6.5	2.54%	24.46%	0.25%	26.56%	27.50%	25.62%
	7	2.67%	26.18%	0.26%	28.34%	29.31%	27.38%
	7.5	2.86%	27.75%	0.26%	30.00%	31.00%	29.01%
	8	2.89%	29.29%	0.26%	31.51%	32.54%	30.49%
	8.5	2.96%	30.36%	0.26%	32.60%	33.66%	31.53%
	9	2.96%	30.86%	0.26%	33.08%	34.18%	31.98%
	1	0.55%	0.13%	0.00%	0.68%	0.93%	0.42%
	1.5	0.70%	0.48%	0.02%	1.20%	1.54%	0.86%
	2	0.80%	1.29%	0.05%	2.13%	2.58%	1.68%
	2.5	0.96%	3.03%	0.08%	4.03%	4.64%	3.42%
	3	1.06%	6.41%	0.13%	7.52%	8.34%	6.71%
	3.5	1.23%	10.92%	0.16%	12.15%	13.17%	11.14%
	4	1.61%	16.48%	0.16%	17.95%	19.14%	16.76%
	4.5	1.76%	21.42%	0.22%	22.98%	24.29%	21.67%
CHILDREN	5	1.93%	25.55%	0.26%	27.17%	28.56%	25.79%
	5.5	2.18%	29.97%	0.26%	31.67%	33.12%	30.22%
	6	2.29%	32.59%	0.29%	34.33%	35.81%	32.85%
	6.5	2.41%	34.77%	0.33%	36.56%	38.06%	35.05%
	7	2.57%	37.61%	0.33%	39.42%	40.98%	37.85%
	7.5	2.73%	39.55%	0.33%	41.40%	43.02%	39.77%
	8	2.82%	41.62%	0.33%	43.46%	45.17%	41.75%
	8.5	3.18%	43.14%	0.33%	45.13%	46.97%	43.29%
	9*	N/A	N/A	N/A	N/A	N/A	N/A

*Sample size is not large enough for reporting.

HIRES 90K ADVANTAGE

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
						CI Higher	CI Lower
ADULTS	1	0.64%	0.06%	0.01%	0.72%	0.83%	0.60%
	2	1.09%	0.08%	0.02%	1.19%	1.34%	1.05%
	3	1.35%	0.13%	0.03%	1.51%	1.68%	1.35%
	4	1.62%	0.17%	0.03%	1.82%	2.00%	1.64%
	5	1.84%	0.19%	0.04%	2.06%	2.26%	1.87%
	6	1.97%	0.22%	0.04%	2.23%	2.44%	2.03%
	7	2.10%	0.23%	0.05%	2.38%	2.59%	2.17%
	8	2.26%	0.27%	0.06%	2.58%	2.80%	2.37%
	9	2.38%	0.33%	0.07%	2.77%	2.99%	2.54%
	10	2.56%	0.33%	0.09%	2.96%	3.20%	2.72%
	11	2.71%	0.35%	0.10%	3.15%	3.40%	2.89%
	12	2.78%	0.36%	0.10%	3.23%	3.49%	2.97%
	13	2.94%	0.44%	0.10%	3.46%	3.79%	3.14%
CHILDREN	1	0.72%	0.19%	0.02%	0.93%	1.06%	0.81%
	2	1.04%	0.35%	0.04%	1.42%	1.58%	1.26%
	3	1.27%	0.56%	0.05%	1.86%	2.04%	1.68%
	4	1.48%	0.71%	0.07%	2.25%	2.45%	2.06%
	5	1.60%	0.85%	0.11%	2.54%	2.74%	2.33%
	6	1.72%	0.97%	0.11%	2.77%	2.99%	2.55%
	7	1.81%	1.05%	0.12%	2.95%	3.18%	2.73%
	8	1.97%	1.19%	0.13%	3.25%	3.50%	3.01%
	9	2.02%	1.26%	0.15%	3.40%	3.66%	3.15%
	10	2.17%	1.35%	0.16%	3.65%	3.92%	3.38%
	11	2.26%	1.37%	0.20%	3.79%	4.07%	3.50%
	12	2.51%	1.37%	0.20%	4.03%	4.36%	3.70%
	13	2.58%	1.37%	0.20%	4.10%	4.45%	3.75%

HIRES 90K vendor A post-mod

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
						CI Higher	CI Lower
ADULTS	1	0.77%	0.07%	0.01%	0.85%	0.94%	0.76%
	2	1.27%	0.11%	0.04%	1.42%	1.54%	1.31%
	3	1.58%	0.16%	0.06%	1.80%	1.93%	1.67%
	4	1.85%	0.24%	0.08%	2.15%	2.29%	2.01%
	5	2.07%	0.27%	0.09%	2.42%	2.57%	2.27%
	6	2.22%	0.33%	0.10%	2.64%	2.80%	2.49%
	7	2.36%	0.35%	0.11%	2.81%	2.97%	2.65%
	8	2.51%	0.42%	0.12%	3.04%	3.20%	2.87%
	9	2.63%	0.47%	0.12%	3.21%	3.38%	3.03%
	10	2.76%	0.50%	0.14%	3.39%	3.57%	3.21%
	11	2.88%	0.54%	0.14%	3.54%	3.73%	3.36%
	12	2.97%	0.55%	0.15%	3.65%	3.84%	3.46%
	13	3.11%	0.58%	0.16%	3.83%	4.02%	3.63%
	14	3.25%	0.60%	0.17%	3.99%	4.19%	3.78%
	15	3.42%	0.61%	0.17%	4.17%	4.39%	3.96%
	16	3.58%	0.65%	0.17%	4.37%	4.60%	4.14%
	17	3.73%	0.71%	0.17%	4.57%	4.82%	4.33%
	18	3.85%	0.76%	0.17%	4.75%	5.01%	4.49%
	19	3.93%	0.84%	0.19%	4.93%	5.21%	4.64%
	20	4.02%	0.84%	0.19%	5.01%	5.32%	4.70%
CHILDREN	1	0.78%	0.19%	0.03%	1.00%	1.10%	0.91%
	2	1.11%	0.45%	0.04%	1.59%	1.71%	1.47%
	3	1.36%	0.72%	0.06%	2.13%	2.27%	1.99%
	4	1.56%	0.97%	0.08%	2.59%	2.75%	2.44%
	5	1.72%	1.18%	0.11%	2.99%	3.15%	2.82%
	6	1.84%	1.34%	0.12%	3.27%	3.44%	3.10%
	7	1.94%	1.45%	0.13%	3.49%	3.67%	3.31%
	8	2.05%	1.61%	0.15%	3.77%	3.95%	3.58%
	9	2.13%	1.71%	0.18%	3.97%	4.16%	3.78%
	10	2.29%	1.87%	0.20%	4.31%	4.51%	4.10%
	11	2.39%	1.89%	0.22%	4.44%	4.65%	4.24%
	12	2.55%	1.95%	0.25%	4.69%	4.90%	4.47%
	13	2.68%	1.98%	0.25%	4.84%	5.07%	4.62%
	14	2.81%	2.05%	0.26%	5.06%	5.29%	4.82%
	15	2.91%	2.10%	0.31%	5.24%	5.49%	4.99%
	16	3.03%	2.19%	0.33%	5.46%	5.74%	5.19%
	17	3.09%	2.22%	0.33%	5.55%	5.83%	5.27%
	18	3.26%	2.30%	0.38%	5.84%	6.16%	5.52%
	19	3.33%	2.37%	0.41%	6.01%	6.36%	5.66%
	20	3.33%	2.61%	0.41%	6.23%	6.67%	5.80%

*Sample size is not large enough for reporting.

HIRES 90K vendor A all

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
						CI Higher	CI Lower
ADULTS	1	0.76%	0.08%	0.01%	0.86%	0.94%	0.77%
	2	1.26%	0.14%	0.05%	1.45%	1.56%	1.33%
	3	1.57%	0.20%	0.08%	1.84%	1.97%	1.71%
	4	1.84%	0.30%	0.09%	2.23%	2.37%	2.08%
	5	2.06%	0.35%	0.11%	2.51%	2.66%	2.36%
	6	2.21%	0.43%	0.12%	2.75%	2.90%	2.59%
	7	2.35%	0.46%	0.14%	2.93%	3.09%	2.77%
	8	2.50%	0.54%	0.14%	3.17%	3.34%	3.00%
	9	2.62%	0.62%	0.15%	3.36%	3.54%	3.19%
	10	2.75%	0.67%	0.17%	3.56%	3.74%	3.38%
	11	2.87%	0.72%	0.17%	3.74%	3.92%	3.55%
	12	2.97%	0.76%	0.18%	3.88%	4.07%	3.69%
	13	3.10%	0.81%	0.19%	4.07%	4.27%	3.87%
	14	3.26%	0.87%	0.19%	4.28%	4.49%	4.07%
	15	3.42%	0.90%	0.19%	4.47%	4.69%	4.25%
	16	3.57%	0.95%	0.20%	4.68%	4.91%	4.45%
	17	3.72%	1.03%	0.21%	4.91%	5.15%	4.66%
	18	3.83%	1.11%	0.21%	5.10%	5.36%	4.84%
	19	3.89%	1.18%	0.23%	5.25%	5.52%	4.97%
	20	4.00%	1.24%	0.23%	5.40%	5.70%	5.10%
	21	4.05%	1.38%	0.23%	5.59%	5.94%	5.24%
	22	4.05%	1.47%	0.23%	5.67%	6.05%	5.28%
CHILDREN	1	0.79%	0.21%	0.03%	1.02%	1.12%	0.93%
	2	1.12%	0.47%	0.04%	1.62%	1.74%	1.50%
	3	1.37%	0.75%	0.06%	2.17%	2.31%	2.04%
	4	1.58%	1.01%	0.08%	2.66%	2.81%	2.50%
	5	1.74%	1.23%	0.12%	3.06%	3.23%	2.90%
	6	1.86%	1.41%	0.13%	3.36%	3.54%	3.19%
	7	1.97%	1.54%	0.14%	3.61%	3.79%	3.44%
	8	2.08%	1.71%	0.17%	3.92%	4.11%	3.73%
	9	2.16%	1.83%	0.19%	4.13%	4.32%	3.93%
	10	2.32%	1.99%	0.22%	4.47%	4.68%	4.27%
	11	2.43%	2.03%	0.24%	4.63%	4.84%	4.42%
	12	2.59%	2.12%	0.26%	4.90%	5.12%	4.68%
	13	2.71%	2.17%	0.26%	5.07%	5.30%	4.84%
	14	2.84%	2.28%	0.28%	5.32%	5.56%	5.08%
	15	2.94%	2.37%	0.32%	5.55%	5.80%	5.29%
	16	3.05%	2.51%	0.34%	5.81%	6.08%	5.53%
	17	3.11%	2.56%	0.34%	5.91%	6.20%	5.63%
	18	3.27%	2.67%	0.38%	6.21%	6.53%	5.89%
	19	3.41%	2.83%	0.41%	6.53%	6.89%	6.16%
	20	3.46%	3.03%	0.46%	6.81%	7.24%	6.38%
	21	3.55%	3.12%	0.46%	6.99%	7.48%	6.50%
	22*	N/A	N/A	N/A	N/A	N/A	N/A

HIRES 90K vendor A pre-mod

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
						CI Higher	CI Lower
ADULTS	1	0.60%	0.42%	0.00%	1.02%	1.51%	0.54%
	2	1.03%	0.85%	0.24%	2.11%	2.80%	1.42%
	3	1.33%	1.09%	0.49%	2.89%	3.70%	2.09%
	4	1.58%	1.89%	0.55%	3.98%	4.92%	3.04%
	5	1.70%	2.33%	0.62%	4.58%	5.59%	3.58%
	6	1.83%	2.76%	0.68%	5.19%	6.25%	4.12%
	7	2.14%	3.01%	0.74%	5.79%	6.91%	4.66%
	8	2.21%	3.57%	0.74%	6.39%	7.57%	5.22%
	9	2.27%	4.25%	0.74%	7.12%	8.35%	5.88%
	10	2.40%	4.62%	0.81%	7.66%	8.94%	6.38%
	11	2.52%	5.00%	0.81%	8.14%	9.46%	6.83%
	12	2.78%	5.44%	0.81%	8.81%	10.18%	7.45%
	13	2.85%	5.69%	0.87%	9.17%	10.56%	7.78%
	14	3.17%	6.13%	0.87%	9.90%	11.34%	8.46%
	15	3.24%	6.32%	0.87%	10.14%	11.60%	8.69%
	16	3.37%	6.45%	0.87%	10.39%	11.85%	8.92%
	17	3.50%	6.70%	0.94%	10.81%	12.31%	9.31%
	18	3.56%	6.89%	0.94%	11.05%	12.56%	9.54%
	19	3.56%	6.95%	0.94%	11.11%	12.63%	9.60%
	20	3.70%	7.08%	0.94%	11.36%	12.89%	9.83%
	21	3.76%	7.27%	0.94%	11.60%	13.15%	10.06%
	22	3.76%	7.36%	0.94%	11.68%	13.23%	10.13%

*Sample size is not large enough for reporting.

HIRES 90K vendor A pre-mod – continued –

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	Total CI Lower
CHILDREN	1	1.24%	0.79%	0.00%	2.03%	2.95%	1.10%
	2	1.47%	1.37%	0.12%	2.93%	4.04%	1.82%
	3	2.05%	2.17%	0.23%	4.40%	5.75%	3.05%
	4	2.40%	3.10%	0.23%	5.65%	7.17%	4.13%
	5	2.52%	3.92%	0.35%	6.67%	8.31%	5.02%
	6	2.63%	4.73%	0.48%	7.68%	9.44%	5.93%
	7	3.12%	5.56%	0.72%	9.16%	11.06%	7.26%
	8	3.72%	6.62%	0.72%	10.74%	12.78%	8.70%
	9	3.72%	6.97%	0.72%	11.08%	13.15%	9.01%
	10	3.85%	7.45%	0.85%	11.76%	13.89%	9.64%
	11	4.22%	7.81%	0.98%	12.56%	14.74%	10.37%
	12	4.22%	8.77%	0.98%	13.47%	15.72%	11.22%
	13	4.22%	9.13%	0.98%	13.81%	16.08%	11.53%
	14	4.22%	9.97%	0.98%	14.61%	16.94%	12.28%
	15	4.47%	10.45%	0.98%	15.29%	17.66%	12.92%
	16	4.47%	11.05%	0.98%	15.86%	18.27%	13.45%
	17	4.47%	11.29%	0.98%	16.09%	18.51%	13.66%
	18	4.60%	11.53%	0.98%	16.43%	18.87%	13.98%
	19	5.00%	12.02%	0.98%	17.23%	19.72%	14.74%
	20	5.13%	12.14%	1.11%	17.57%	20.08%	15.06%
	21	5.13%	12.14%	1.11%	17.57%	20.08%	15.06%
	22*	N/A	N/A	N/A	N/A	N/A	N/A

HIRES 90K vendor B

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	Total CI Lower
ADULTS	1	0.95%	3.03%	0.00%	3.95%	4.71%	3.20%
	2	1.33%	10.84%	0.09%	12.11%	13.37%	10.84%
	3	1.56%	16.19%	0.18%	17.65%	19.12%	16.17%
	4	1.85%	20.73%	0.18%	22.34%	23.95%	20.72%
	5	1.95%	24.36%	0.23%	26.01%	27.72%	24.31%
	6	2.06%	26.71%	0.23%	28.39%	30.14%	26.63%
	7	2.17%	29.67%	0.23%	31.36%	33.16%	29.55%
	8	2.46%	31.54%	0.23%	33.38%	35.21%	31.54%
	9	2.46%	33.13%	0.23%	34.93%	36.78%	33.07%
	10	2.64%	34.56%	0.23%	36.44%	38.31%	34.56%
	11	2.64%	35.51%	0.23%	37.35%	39.23%	35.47%
	12	2.70%	36.82%	0.23%	38.67%	40.56%	36.77%
	13	2.76%	37.85%	0.23%	39.71%	41.61%	37.80%
	14	2.89%	38.63%	0.23%	40.54%	42.46%	38.63%
	15	2.96%	39.29%	0.23%	41.22%	43.14%	39.31%
	16	3.03%	39.79%	0.23%	41.74%	43.67%	39.82%
	17	3.09%	40.58%	0.23%	42.55%	44.47%	40.62%
	18	3.16%	40.99%	0.23%	42.99%	44.92%	41.06%
	19	3.37%	41.53%	0.23%	43.63%	45.57%	41.70%
	20	3.64%	41.99%	0.23%	44.24%	46.17%	42.30%
	21	3.74%	42.28%	0.23%	44.57%	46.52%	42.63%
	22*	N/A	N/A	N/A	N/A	N/A	N/A
CHILDREN	1	0.88%	3.28%	0.00%	4.13%	5.13%	3.12%
	2	1.31%	11.51%	0.07%	12.73%	14.42%	11.05%
	3	1.55%	19.79%	0.07%	21.10%	23.16%	19.03%
	4	1.55%	25.80%	0.07%	27.01%	29.26%	24.76%
	5	1.93%	30.47%	0.17%	31.92%	34.29%	29.56%
	6	2.13%	34.39%	0.17%	35.90%	38.33%	33.46%
	7	2.13%	37.64%	0.17%	39.07%	41.54%	36.59%
	8	2.35%	40.26%	0.17%	41.76%	44.27%	39.26%
	9	2.46%	42.62%	0.17%	44.13%	46.65%	41.61%
	10	2.46%	44.29%	0.17%	45.75%	48.28%	43.22%
	11	2.71%	45.40%	0.17%	46.97%	49.51%	44.43%
	12	3.08%	46.24%	0.42%	48.12%	50.66%	45.58%
	13	3.08%	47.78%	0.42%	49.61%	52.15%	47.07%
	14	3.21%	48.34%	0.56%	50.29%	52.83%	47.74%
	15	3.21%	49.26%	0.56%	51.17%	53.71%	48.63%
	16	3.21%	49.54%	0.70%	51.51%	54.05%	48.97%
	17	3.49%	50.25%	0.70%	52.32%	54.86%	49.78%
	18	3.63%	50.96%	0.70%	53.07%	55.61%	50.53%
	19	4.19%	51.75%	0.70%	54.09%	56.63%	51.56%
	20	4.33%	52.39%	0.70%	54.78%	57.31%	52.25%
	21*	N/A	N/A	N/A	N/A	N/A	N/A
	22*	N/A	N/A	N/A	N/A	N/A	N/A

*Sample size is not large enough for reporting.

CII BIONIC EAR

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	Total CI Lower
ADULTS	1	0.38%	0.38%	0.03%	0.80%	1.10%	0.50%
	2	0.65%	0.41%	0.18%	1.24%	1.61%	0.87%
	3	0.89%	0.59%	0.30%	1.77%	2.21%	1.33%
	4	1.19%	0.65%	0.39%	2.21%	2.71%	1.72%
	5	1.37%	0.74%	0.42%	2.51%	3.03%	1.98%
	6	1.46%	0.89%	0.48%	2.80%	3.36%	2.25%
	7	1.58%	0.95%	0.66%	3.16%	3.75%	2.57%
	8	1.70%	1.04%	0.75%	3.46%	4.07%	2.84%
	9	1.91%	1.14%	0.81%	3.81%	4.46%	3.17%
	10	2.03%	1.20%	0.81%	3.99%	4.65%	3.33%
	11	2.12%	1.29%	0.84%	4.20%	4.87%	3.52%
	12	2.33%	1.29%	0.87%	4.43%	5.13%	3.74%
	13	2.39%	1.29%	0.87%	4.49%	5.19%	3.79%
	14	2.45%	1.38%	0.87%	4.64%	5.35%	3.93%
	15	2.54%	1.44%	0.87%	4.79%	5.51%	4.07%
	16	2.61%	1.50%	0.87%	4.91%	5.64%	4.18%
	17	2.67%	1.57%	0.87%	5.03%	5.76%	4.29%
	18	2.76%	1.60%	0.94%	5.21%	5.95%	4.46%
	19	2.85%	1.66%	0.94%	5.35%	6.11%	4.60%
	20	3.03%	1.66%	0.97%	5.56%	6.34%	4.79%
	21	3.12%	1.69%	1.03%	5.74%	6.53%	4.96%
	22	3.40%	1.72%	1.06%	6.07%	6.88%	5.27%
	23	3.77%	1.75%	1.10%	6.49%	7.33%	5.66%
	24	3.95%	1.75%	1.10%	6.67%	7.52%	5.82%
CHILDREN	1	0.23%	0.76%	0.06%	1.05%	1.53%	0.57%
	2	0.71%	1.40%	0.24%	2.33%	3.05%	1.62%
	3	1.30%	2.29%	0.30%	3.85%	4.76%	2.94%
	4	1.30%	2.77%	0.42%	4.44%	5.41%	3.46%
	5	1.61%	3.25%	0.72%	5.49%	6.57%	4.41%
	6	1.85%	4.03%	1.03%	6.78%	7.97%	5.59%
	7	1.98%	4.57%	1.16%	7.54%	8.79%	6.29%
	8	2.10%	5.00%	1.47%	8.36%	9.67%	7.05%
	9	2.29%	5.42%	1.60%	9.07%	10.43%	7.70%
	10	2.48%	5.79%	1.60%	9.59%	10.99%	8.20%
	11	2.61%	5.91%	1.79%	10.00%	11.43%	8.58%
	12	2.92%	6.03%	1.86%	10.47%	11.93%	9.02%
	13	3.24%	6.16%	1.92%	10.94%	12.43%	9.46%
	14	3.37%	6.41%	1.99%	11.36%	12.86%	9.85%
	15	3.44%	6.47%	1.99%	11.47%	12.99%	9.96%
	16	3.63%	6.53%	2.05%	11.77%	13.30%	10.24%
	17	3.89%	6.59%	2.18%	12.18%	13.73%	10.63%
	18	3.95%	6.72%	2.25%	12.42%	13.98%	10.85%
	19	4.53%	6.91%	2.25%	13.12%	14.73%	11.52%
	20	4.73%	6.91%	2.38%	13.42%	15.04%	11.80%
	21	4.73%	6.91%	2.38%	13.42%	15.04%	11.80%
	22	4.93%	6.91%	2.45%	13.67%	15.30%	12.03%
	23	5.01%	6.91%	2.45%	13.74%	15.37%	12.10%
	24	5.22%	7.01%	2.45%	14.03%	15.69%	12.36%

*Sample size is not large enough for reporting.

CLARION 1.2

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
						CI Higher	CI Lower
	1	0.28%	0.28%	0.14%	0.70%	0.93%	0.47%
	2	0.38%	0.58%	0.24%	1.21%	1.51%	0.90%
	3	0.57%	1.26%	0.34%	2.15%	2.56%	1.75%
	4	0.77%	2.34%	0.51%	3.59%	4.10%	3.07%
	5	0.92%	3.61%	0.66%	5.12%	5.73%	4.51%
	6	1.09%	4.61%	0.74%	6.35%	7.03%	5.67%
	7	1.15%	5.50%	0.83%	7.36%	8.09%	6.64%
	8	1.35%	6.68%	0.96%	8.82%	9.61%	8.03%
	9	1.50%	7.38%	1.09%	9.77%	10.60%	8.95%
	10	1.75%	8.30%	1.29%	11.07%	11.95%	10.20%
	11	1.91%	9.04%	1.38%	12.01%	12.91%	11.10%
	12	2.20%	9.52%	1.59%	12.92%	13.86%	11.99%
	13	2.39%	9.97%	1.64%	13.55%	14.51%	12.60%
	14	2.57%	10.35%	1.73%	14.16%	15.13%	13.19%
ADULTS	15	2.85%	10.77%	1.80%	14.88%	15.87%	13.88%
	16	3.20%	11.14%	1.87%	15.59%	16.60%	14.58%
	17	3.62%	11.57%	1.94%	16.43%	17.46%	15.39%
	18	4.35%	11.92%	1.94%	17.39%	18.44%	16.33%
	19	4.83%	12.25%	2.04%	18.18%	19.26%	17.11%
	20	5.42%	12.47%	2.11%	18.96%	20.06%	17.87%
	21	5.93%	12.64%	2.16%	19.60%	20.71%	18.49%
	22	6.19%	12.87%	2.26%	20.11%	21.23%	18.99%
	23	6.88%	13.14%	2.26%	20.94%	22.08%	19.81%
	24	7.30%	13.35%	2.34%	21.56%	22.71%	20.41%
	25	7.93%	13.50%	2.37%	22.24%	23.40%	21.07%
	26	8.69%	13.67%	2.37%	23.04%	24.22%	21.85%
	27	9.52%	13.92%	2.46%	24.03%	25.26%	22.80%
	28	10.15%	13.98%	2.54%	24.67%	25.95%	23.40%
	29	10.89%	14.22%	2.54%	25.50%	26.88%	24.12%
	1	0.23%	1.68%	0.11%	2.02%	2.48%	1.55%
	2	0.38%	3.09%	0.20%	3.65%	4.27%	3.03%
	3	0.53%	5.25%	0.41%	6.14%	6.94%	5.34%
	4	0.80%	7.64%	0.54%	8.87%	9.81%	7.93%
	5	0.96%	9.95%	0.92%	11.64%	12.70%	10.57%
	6	1.26%	12.43%	1.22%	14.58%	15.75%	13.41%
	7	1.63%	14.30%	1.49%	16.95%	18.20%	15.71%
	8	1.91%	16.43%	1.84%	19.53%	20.85%	18.22%
	9	2.23%	17.77%	2.26%	21.42%	22.79%	20.06%
	10	2.49%	19.36%	2.81%	23.57%	24.99%	22.16%
	11	2.75%	20.47%	3.19%	25.12%	26.56%	23.68%
	12	2.98%	21.18%	3.45%	26.17%	27.63%	24.71%
	13	3.25%	21.84%	3.68%	27.16%	28.65%	25.68%
	14	3.56%	22.47%	3.80%	28.07%	29.57%	26.57%
CHILDREN	15	4.08%	23.61%	4.04%	29.68%	31.21%	28.16%
	16	4.84%	24.44%	4.36%	31.24%	32.79%	29.69%
	17	5.42%	25.10%	4.77%	32.54%	34.10%	30.97%
	18	6.50%	25.72%	4.98%	34.02%	35.60%	32.43%
	19	7.73%	26.23%	5.16%	35.44%	37.04%	33.84%
	20	9.14%	26.61%	5.33%	36.87%	38.48%	35.26%
	21	10.09%	27.06%	5.61%	38.10%	39.72%	36.47%
	22	11.36%	27.74%	5.79%	39.66%	41.30%	38.02%
	23	12.30%	28.03%	5.89%	40.61%	42.25%	38.96%
	24	13.87%	28.54%	5.99%	42.14%	43.80%	40.48%
	25	15.00%	29.05%	6.10%	43.38%	45.05%	41.70%
	26	16.17%	29.83%	6.38%	44.93%	46.62%	43.23%
	27	17.92%	30.05%	6.48%	46.30%	48.05%	44.56%
	28	18.76%	30.41%	6.48%	47.13%	48.92%	45.33%
	29*	N/A	N/A	N/A	N/A	N/A	N/A

*Sample size is not large enough for reporting.

CONTACT US

This report is intended to provide both professionals and our CI recipients with relevant information on the reliability of our products. If you have any questions, please contact us by emailing hear@AdvancedBionics.com or visit our website AdvancedBionics.com for more general information.

ADVANCED BIONICS
POWERFUL CONNECTIONS

ADVANCED BIONICS LLC
28515 Westinghouse Place
Valencia, CA 91355, United States
T: +1.877.829.0026
T: +1.661.362.1400
F: +1.661.362.1500
info.us@advancedbionics.com

ADVANCED BIONICS AG
Laubisrütistrasse 28
8712 Stäfa, Switzerland
T: +41.58.928.78.00
F: +41.58.928.78.90
info.switzerland@advancedbionics.com

For information on additional AB locations, please visit *advancedbionics.com/contact*

Advanced Bionics – A Sonova brand

Please contact your local AB representative for regulatory approval and availability in your region.

ADVANCED
BIONICS

028-Q048-02 Rev H